

FIG. 1

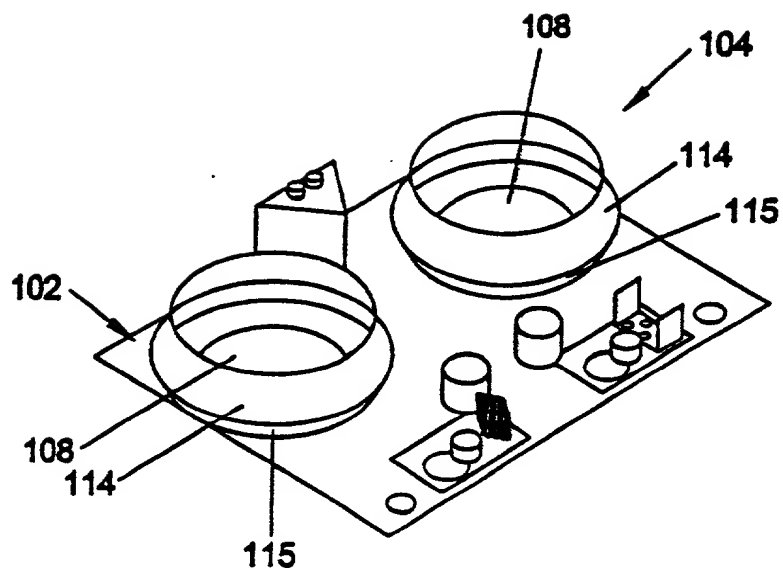


FIG. 2

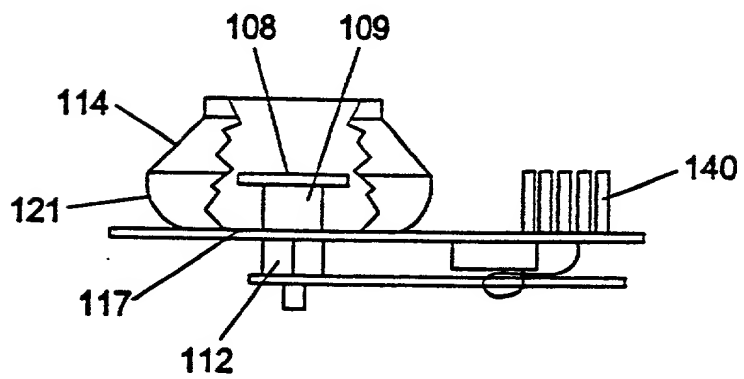


FIG. 3

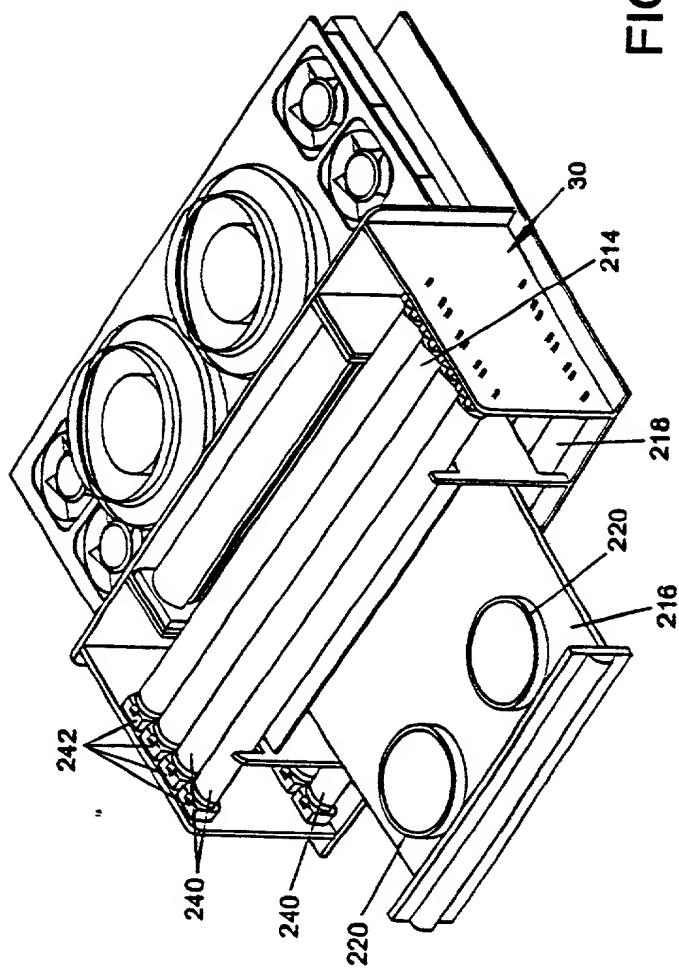


FIG. 4

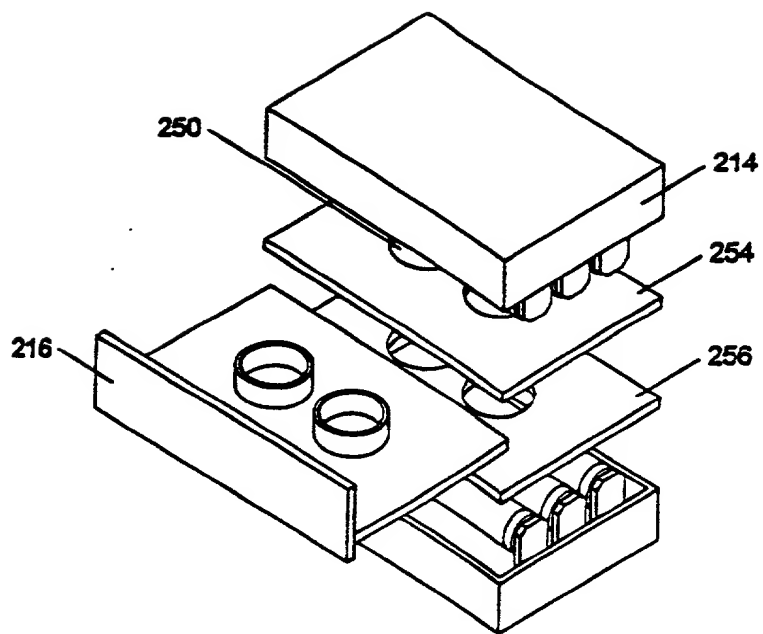


FIG. 5

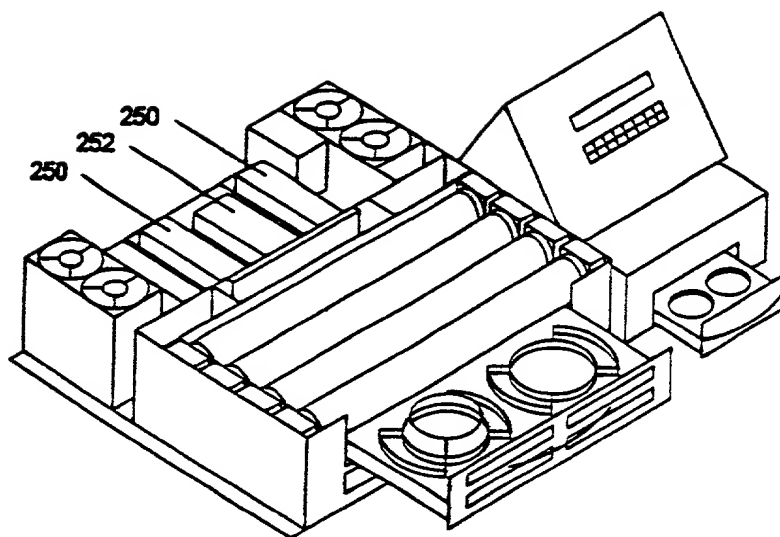


FIG. 6

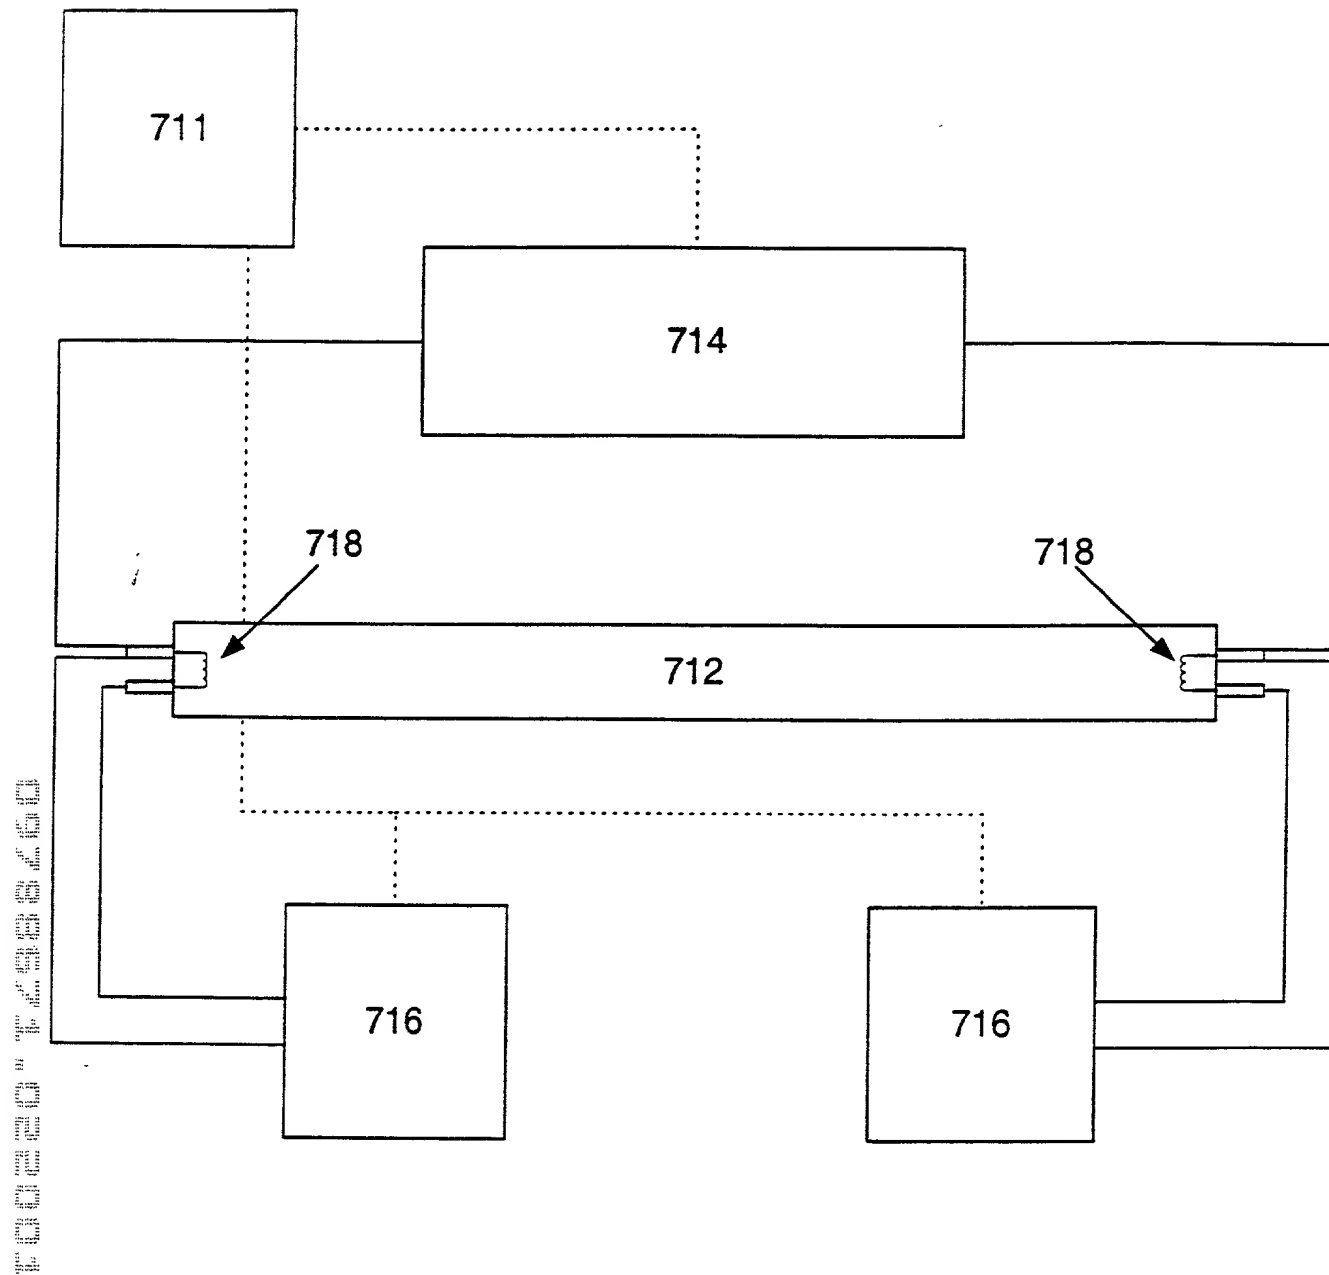


FIG. 7

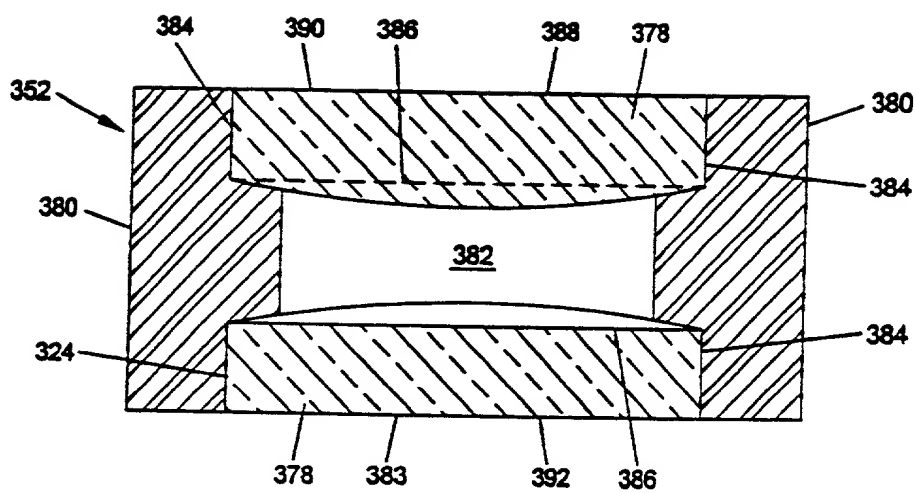
[illegible]

FIG. 8

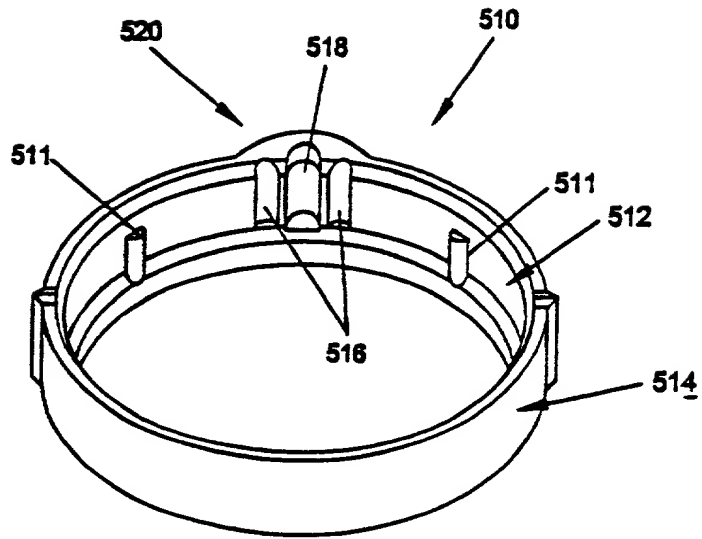


FIG. 9

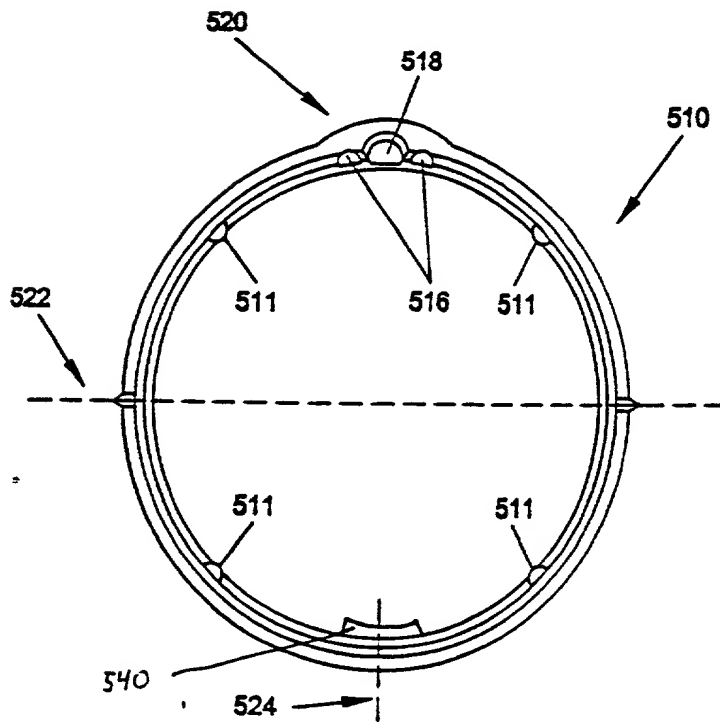


FIG. 10

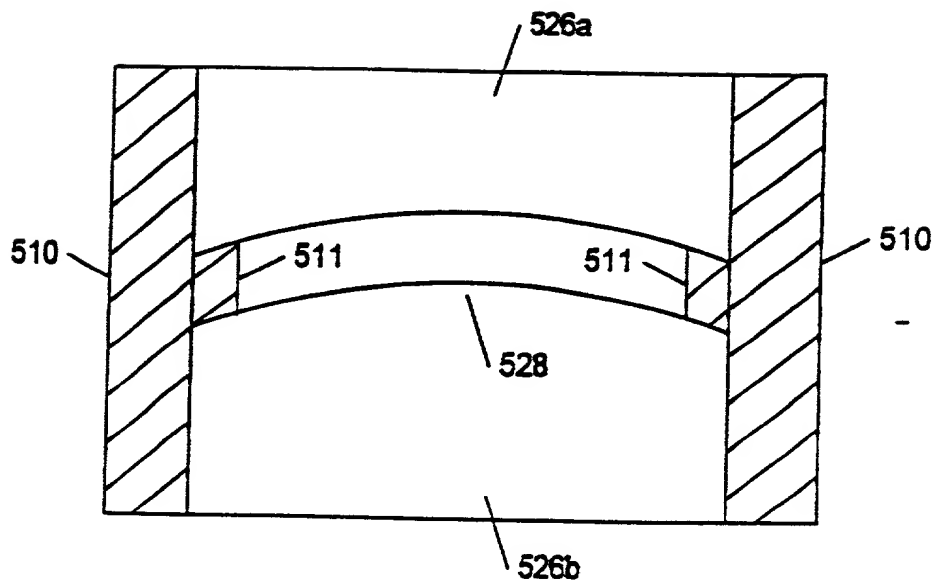


FIG. 11

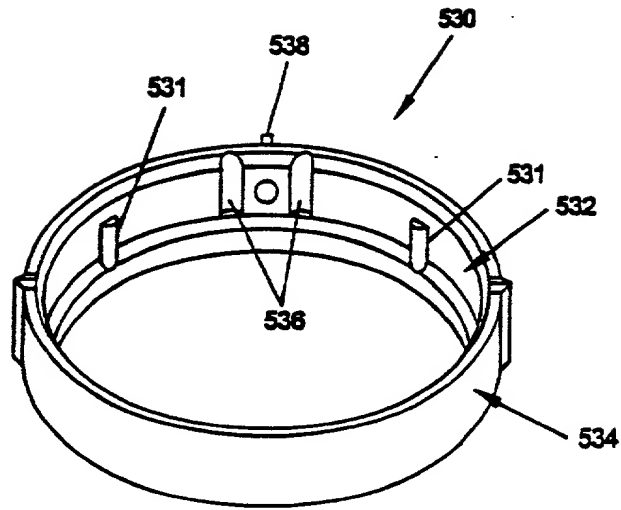


FIG. 12

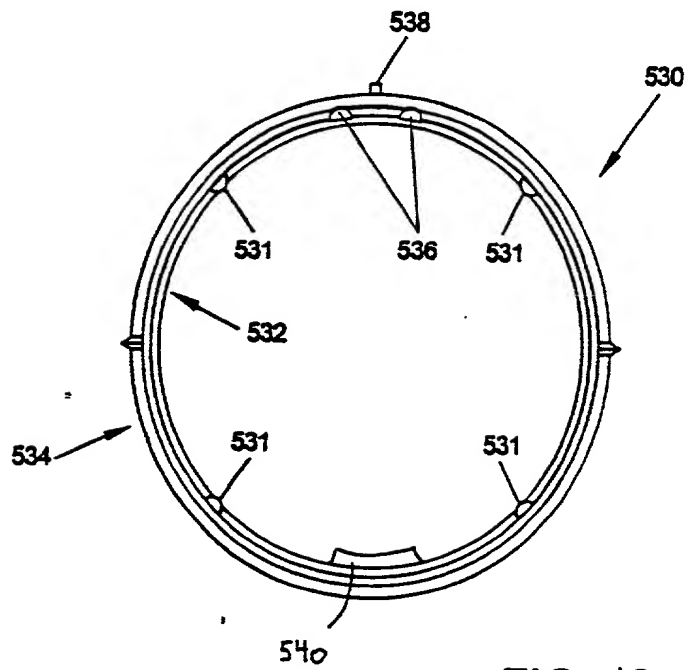


FIG. 13

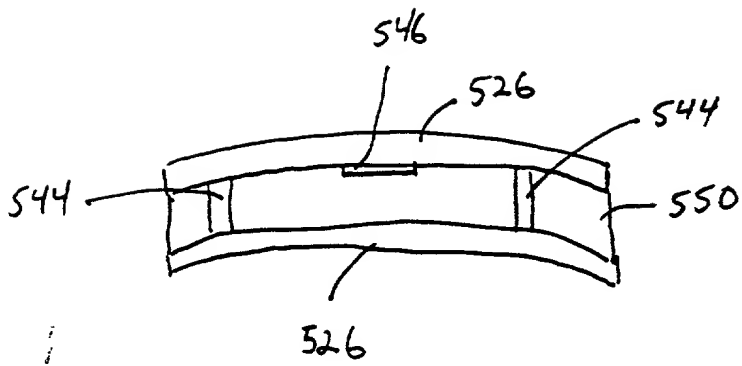


FIG. 14

Downloaded from www.ascelibrary.org

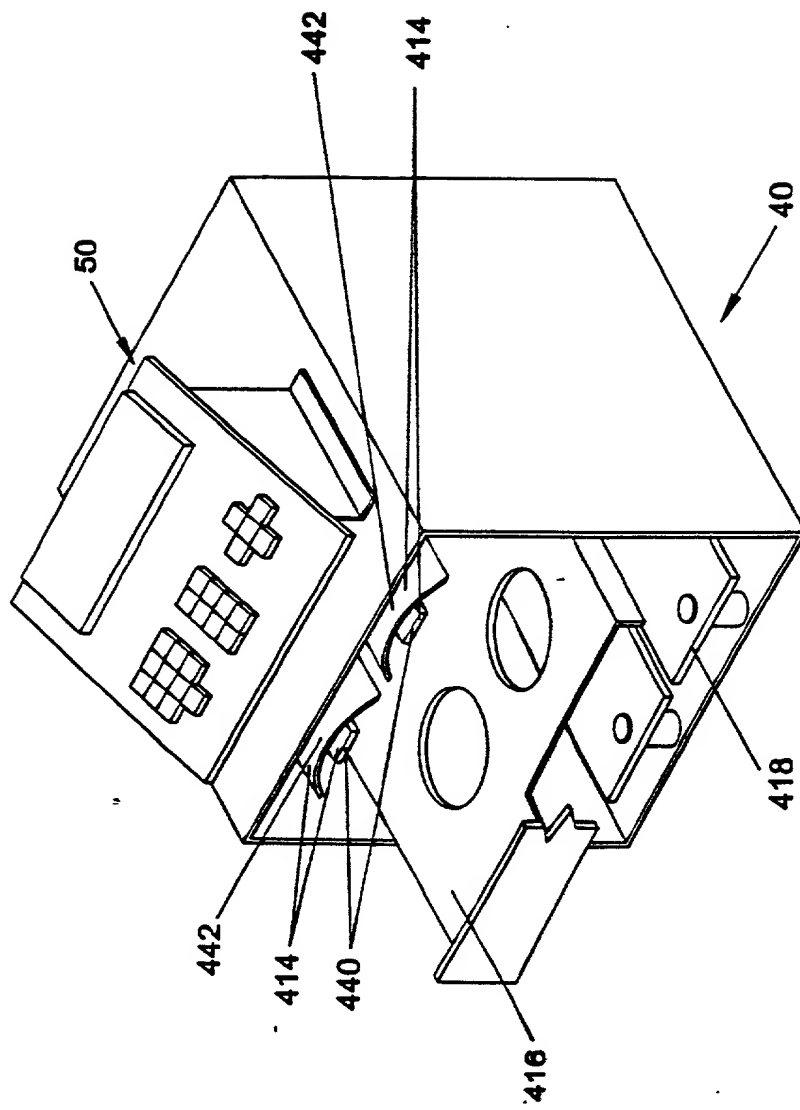


FIG. 15

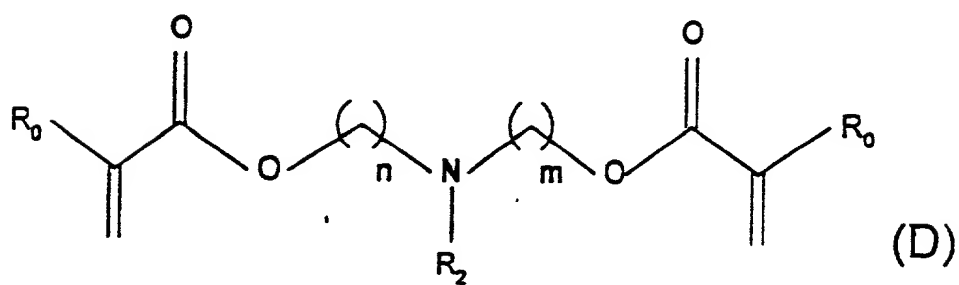
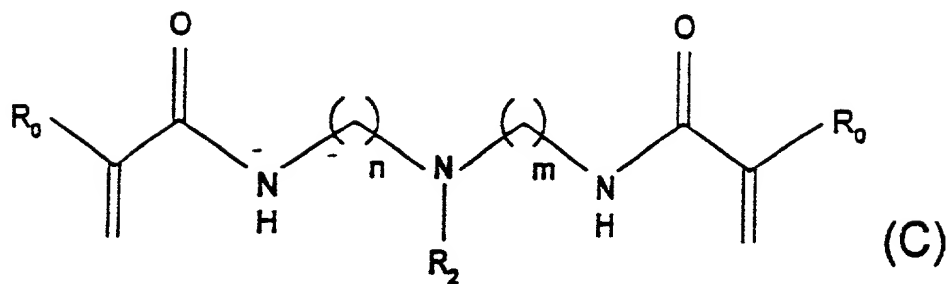
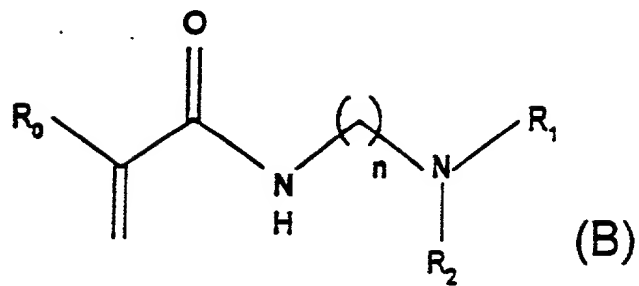
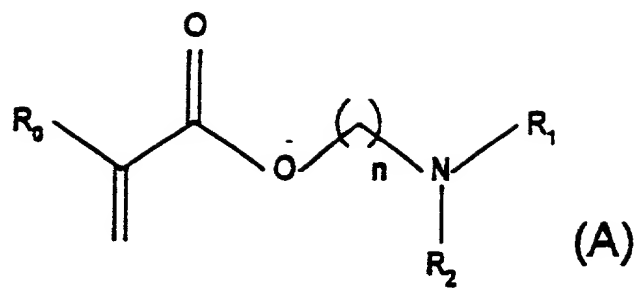


FIG. 16

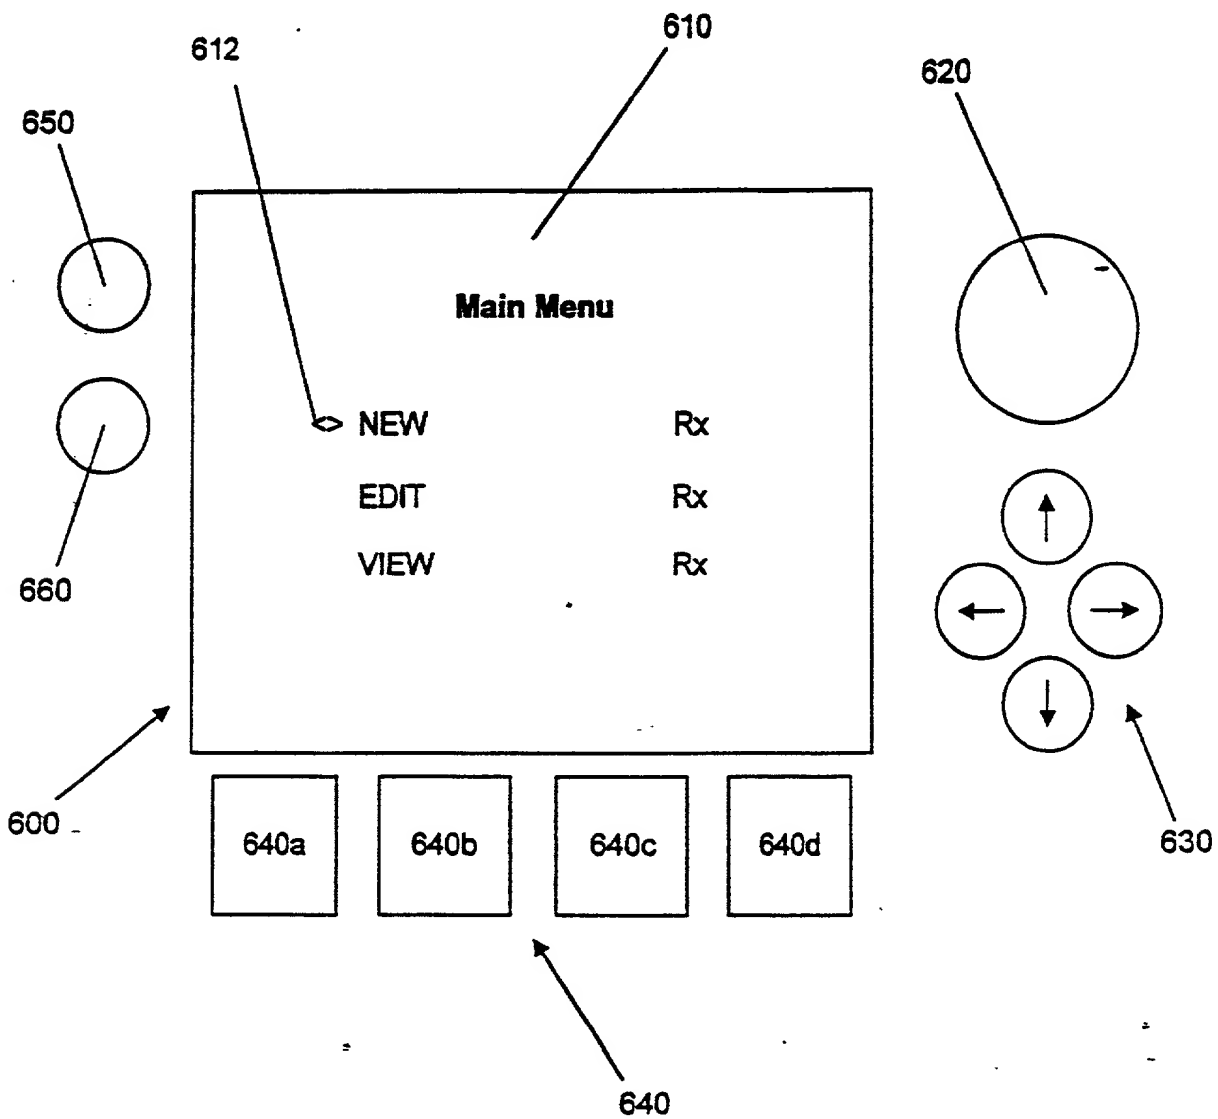


FIG. 17

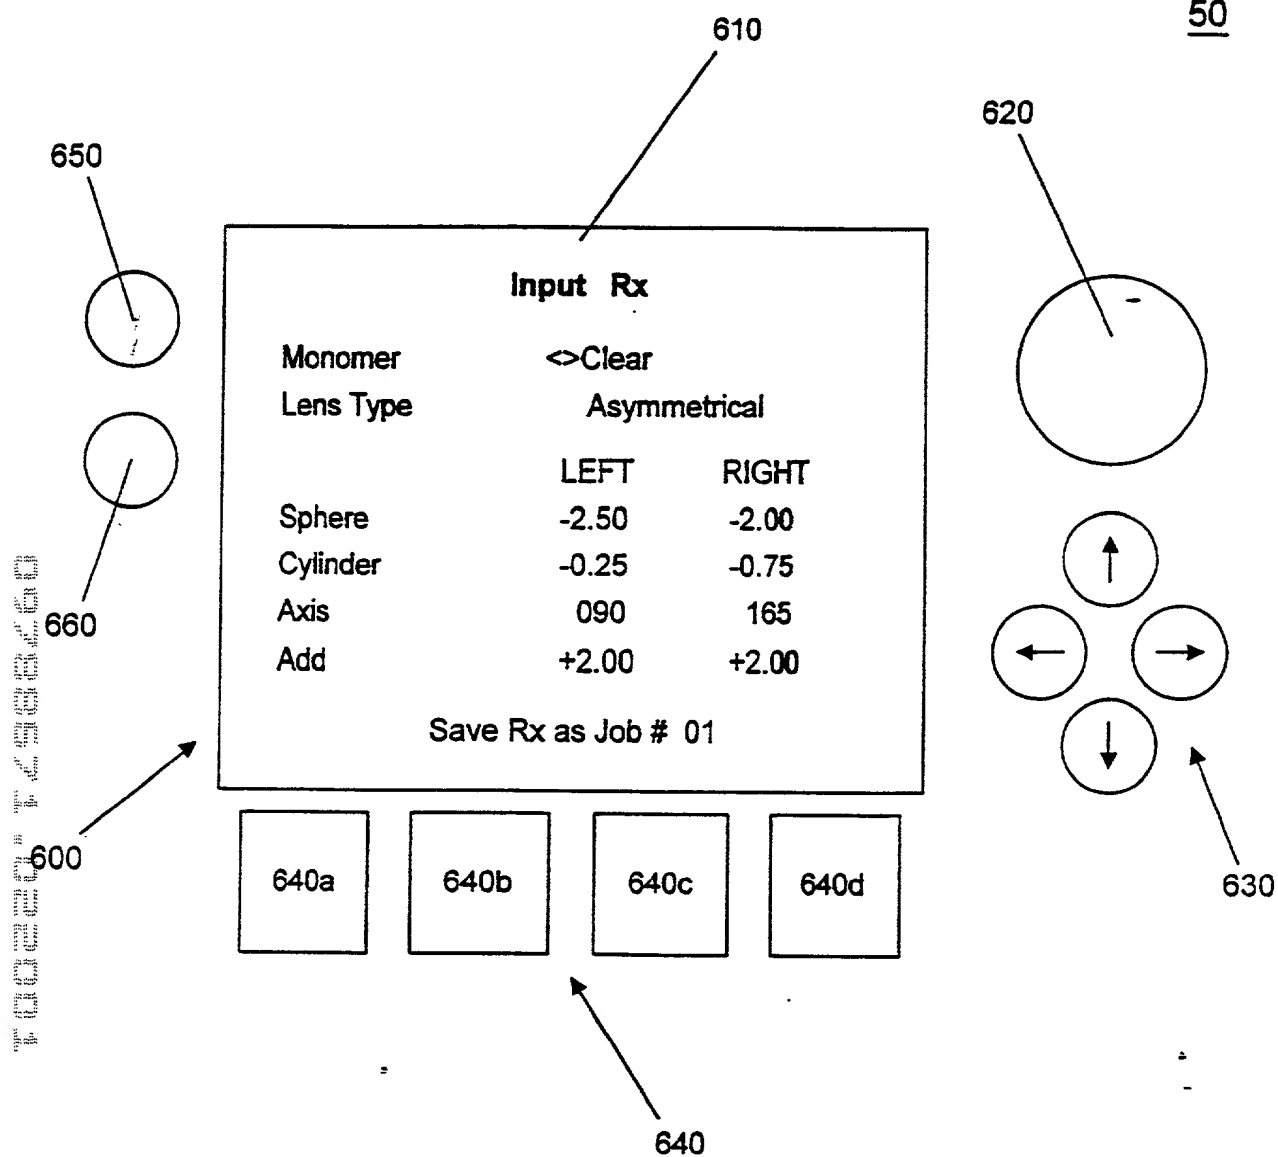


FIG. 18

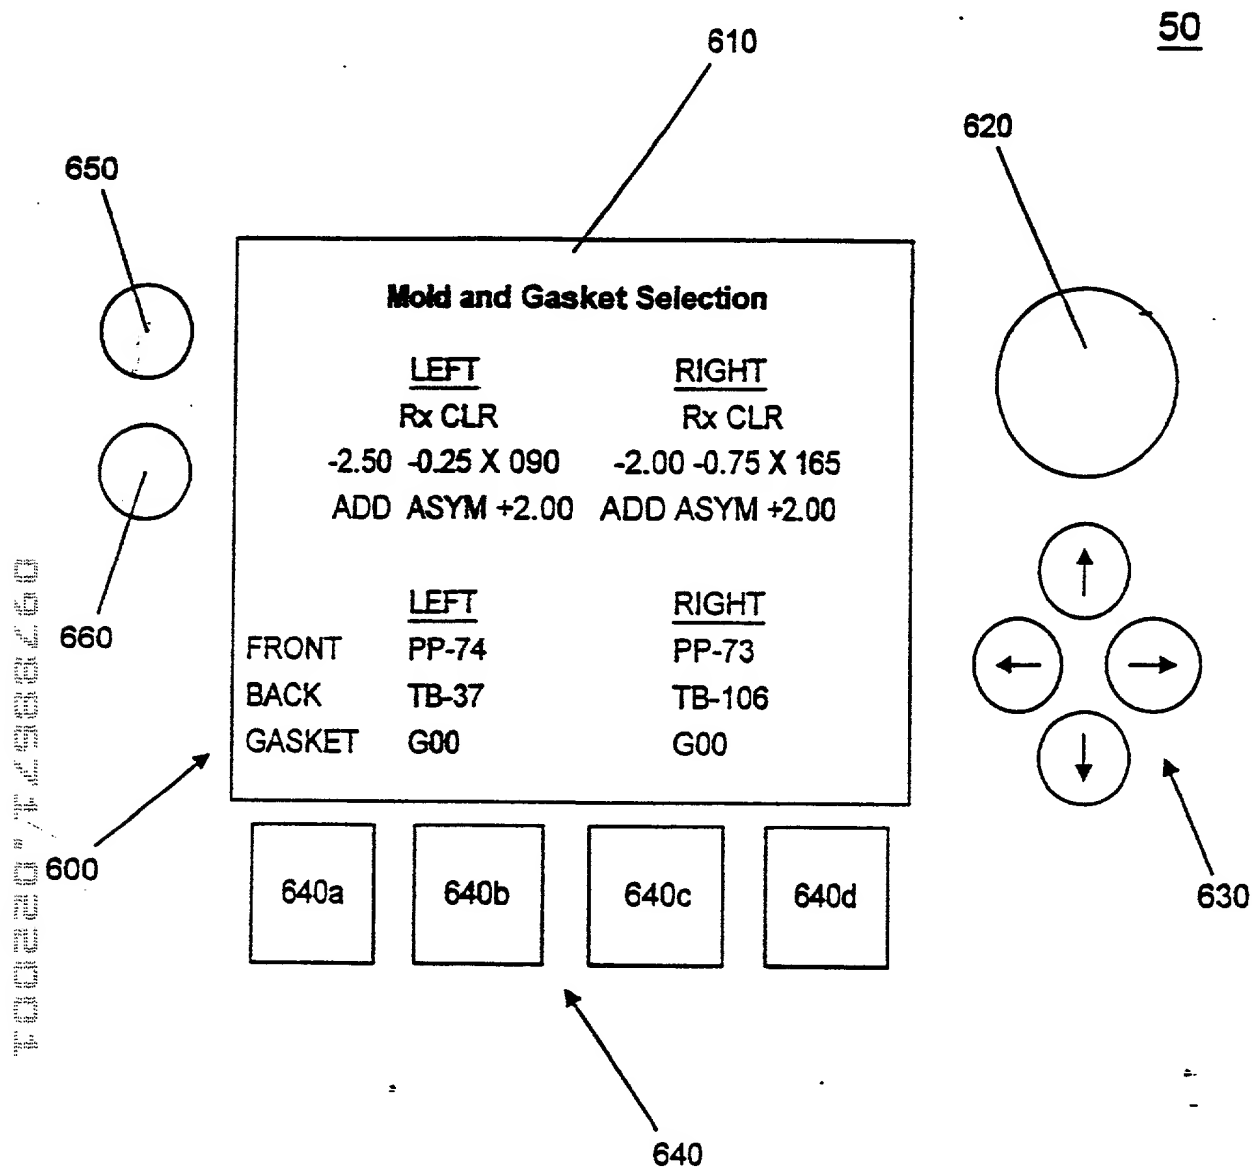
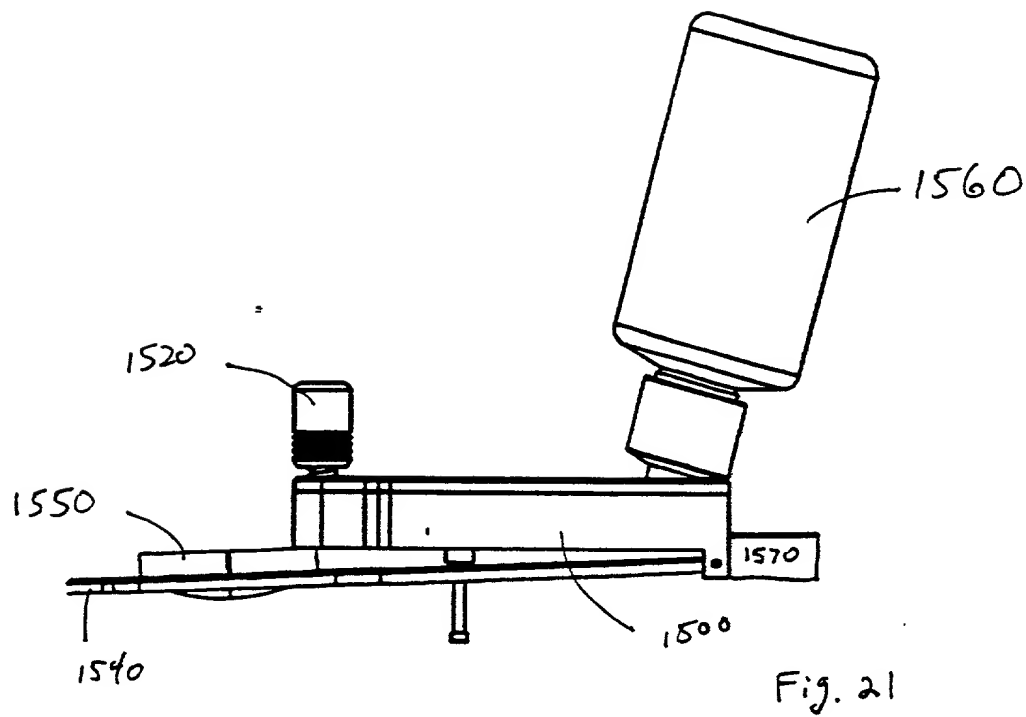
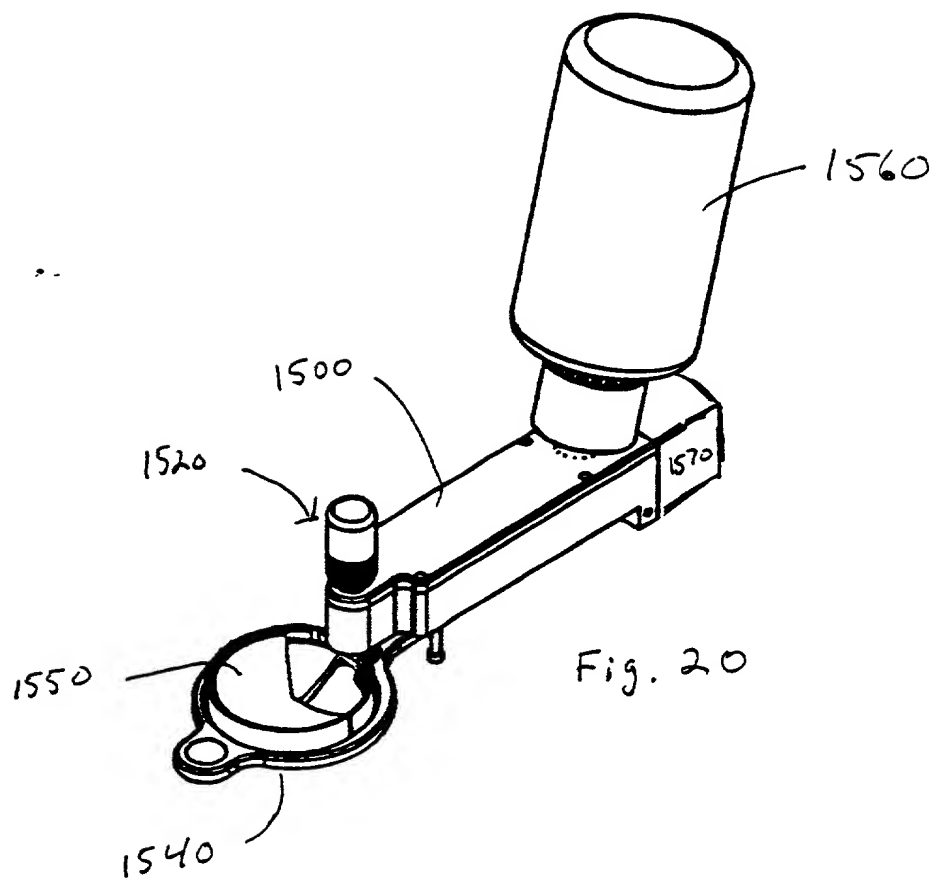
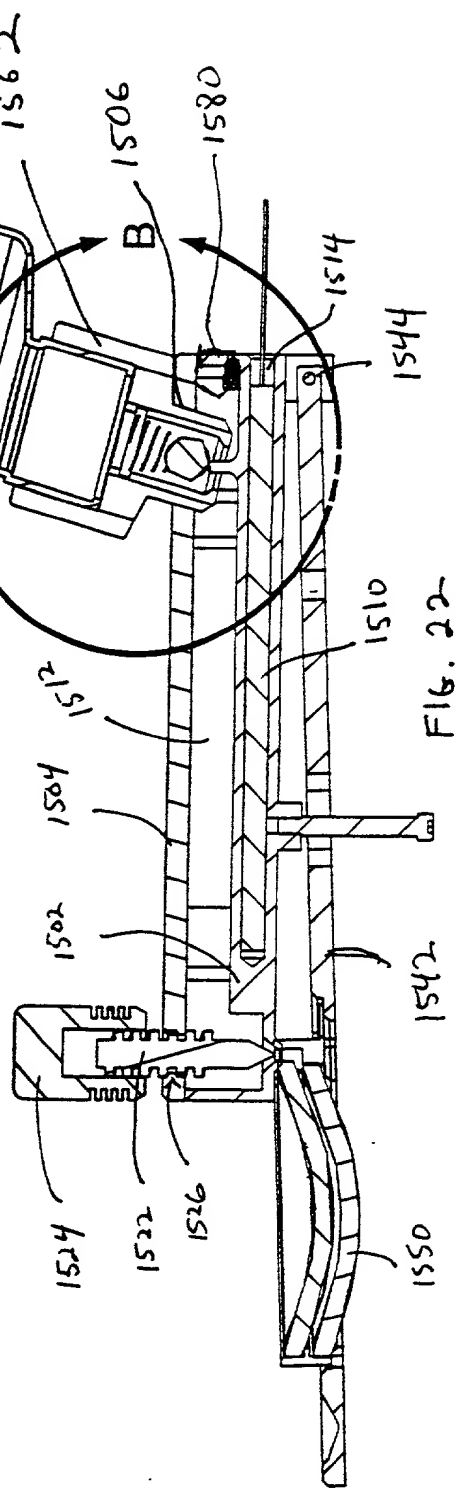
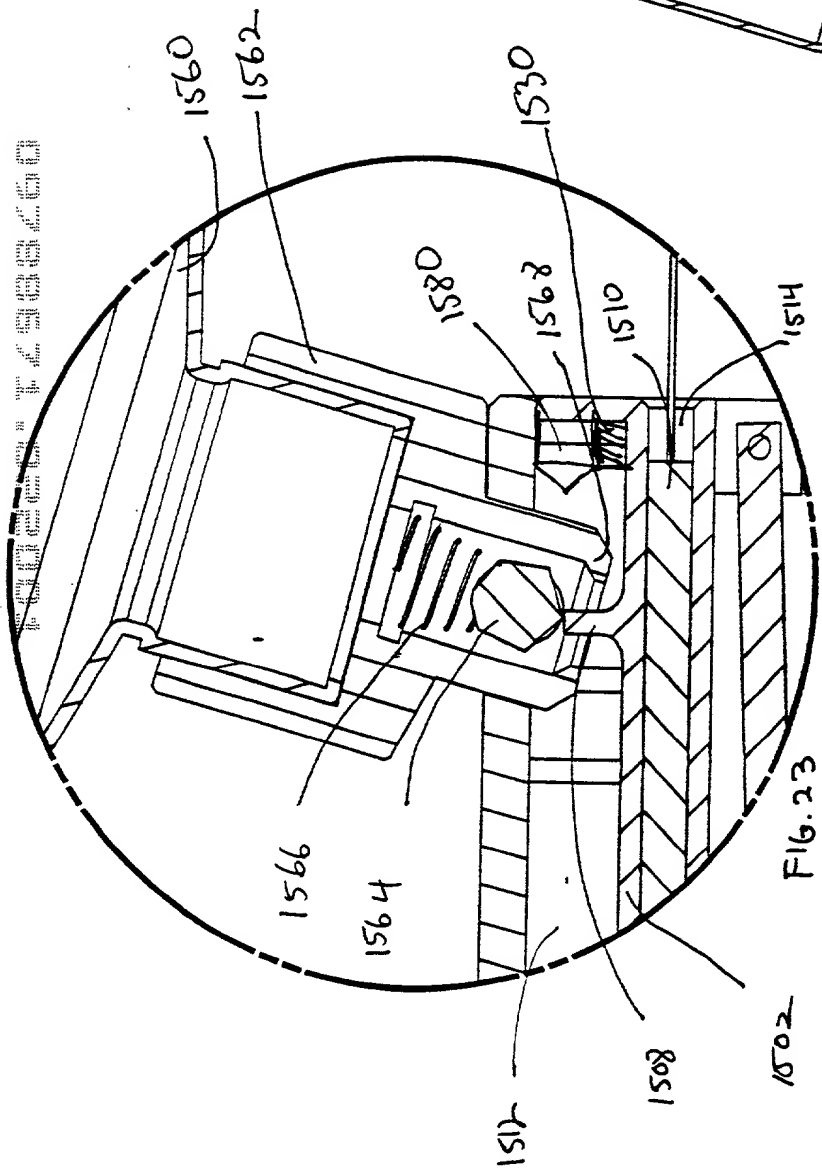


FIG. 19





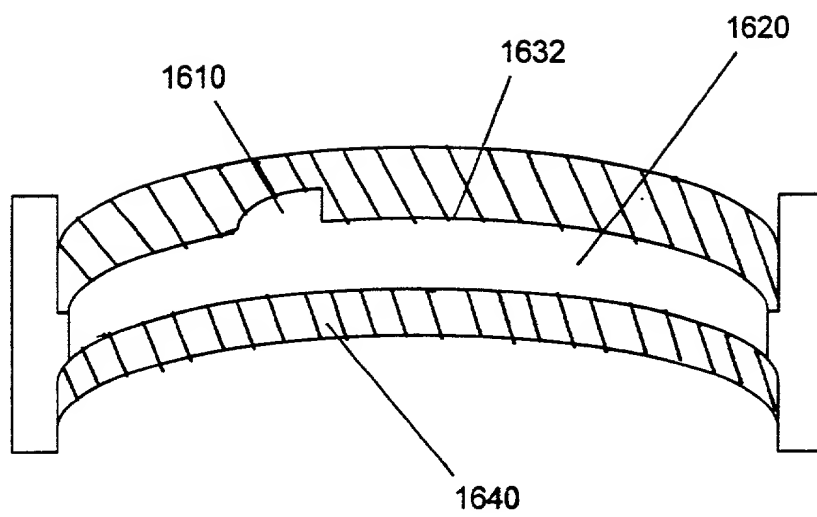


FIG. 24

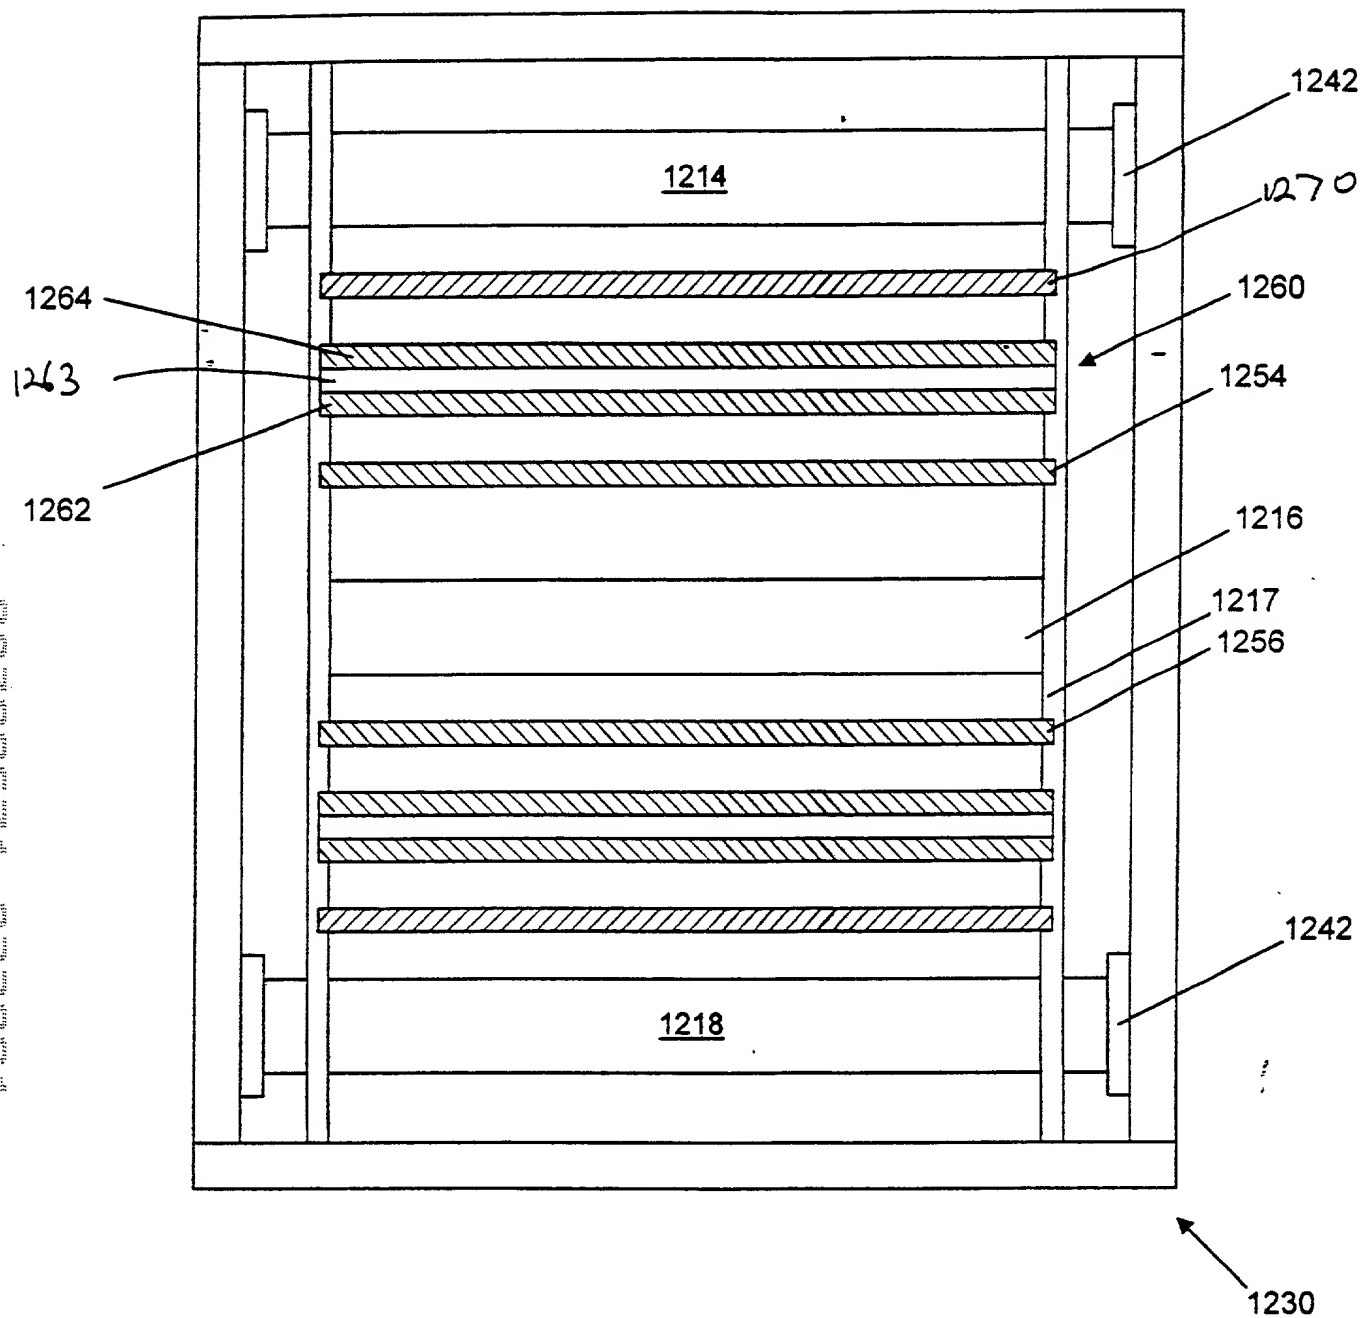


FIG. 25

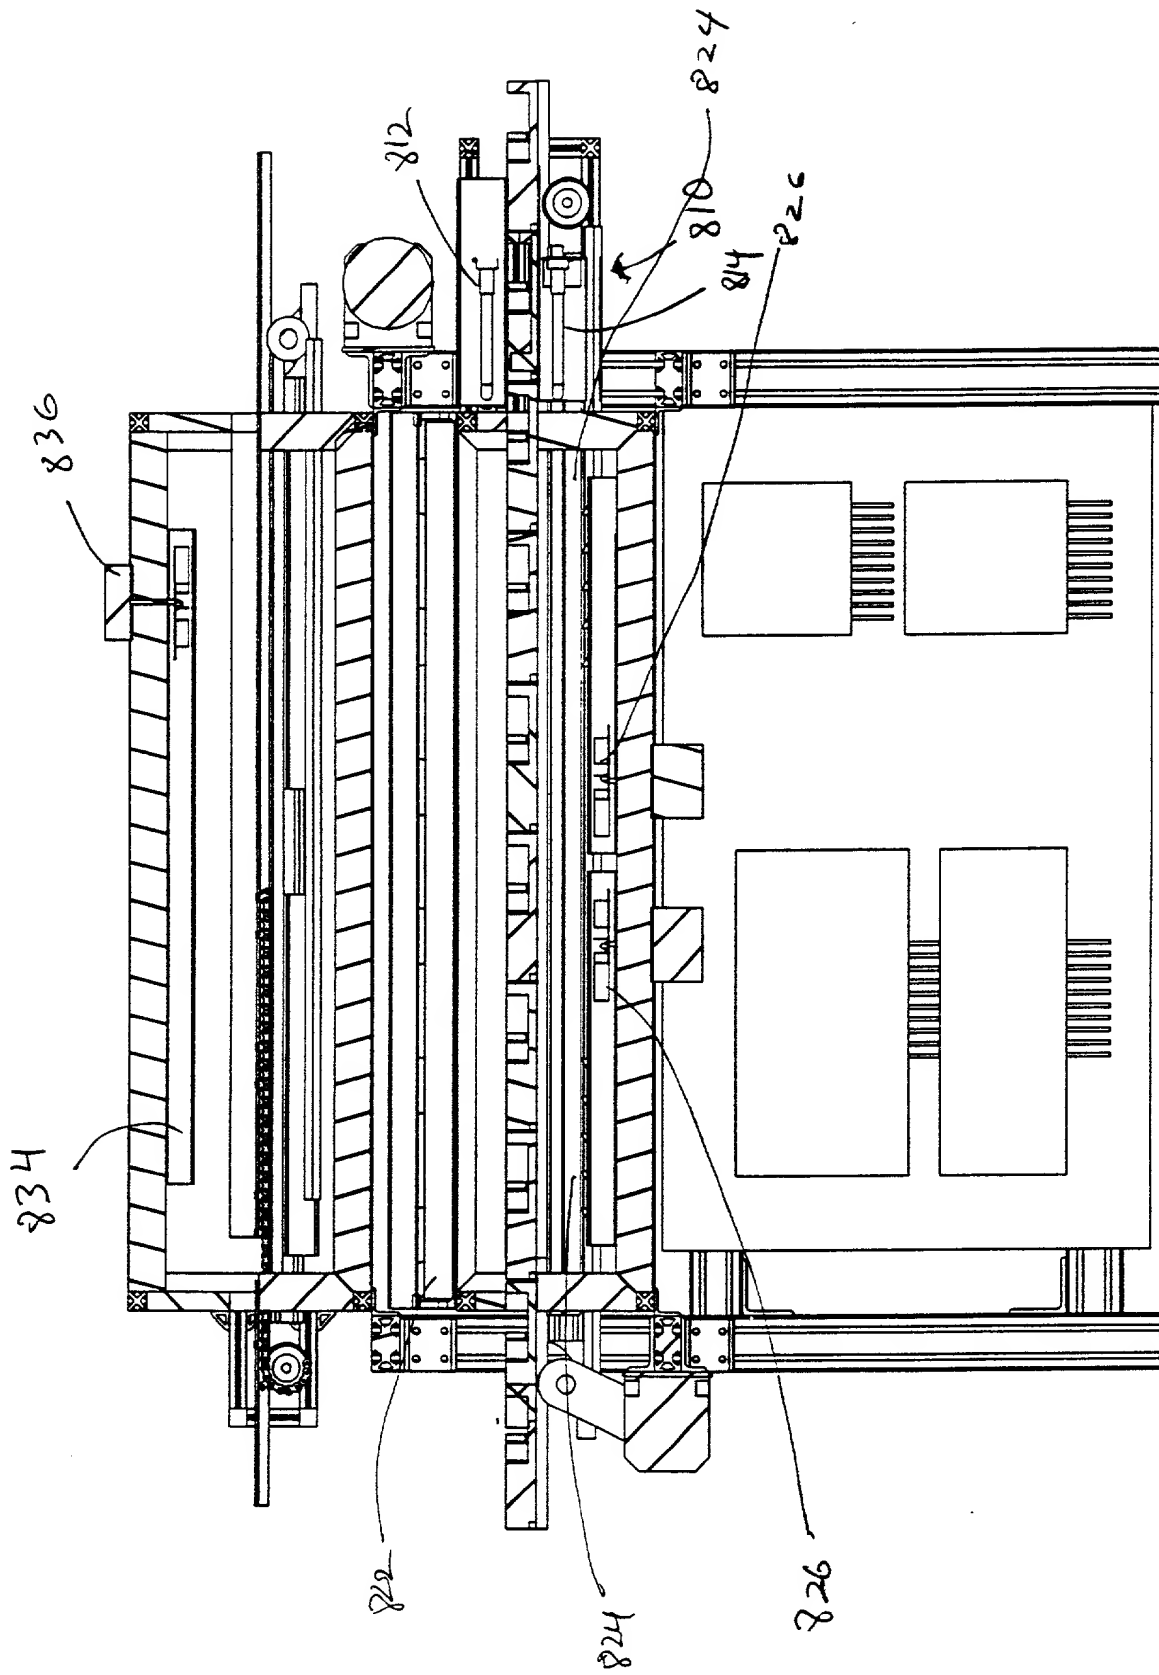


FIG. 28

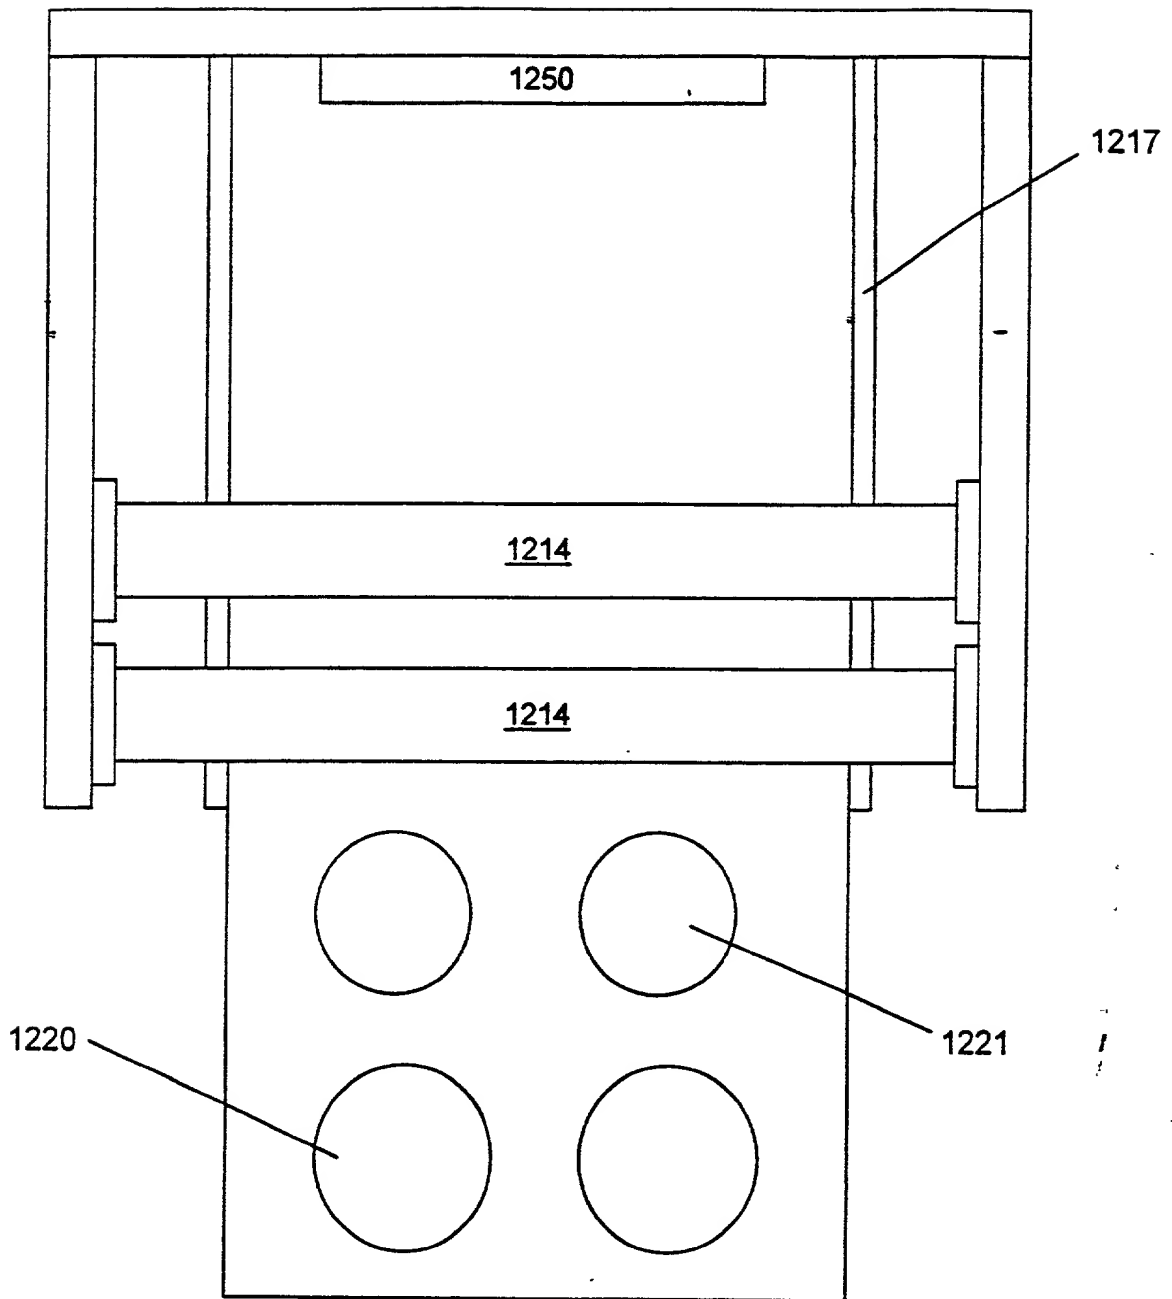


FIG. 26

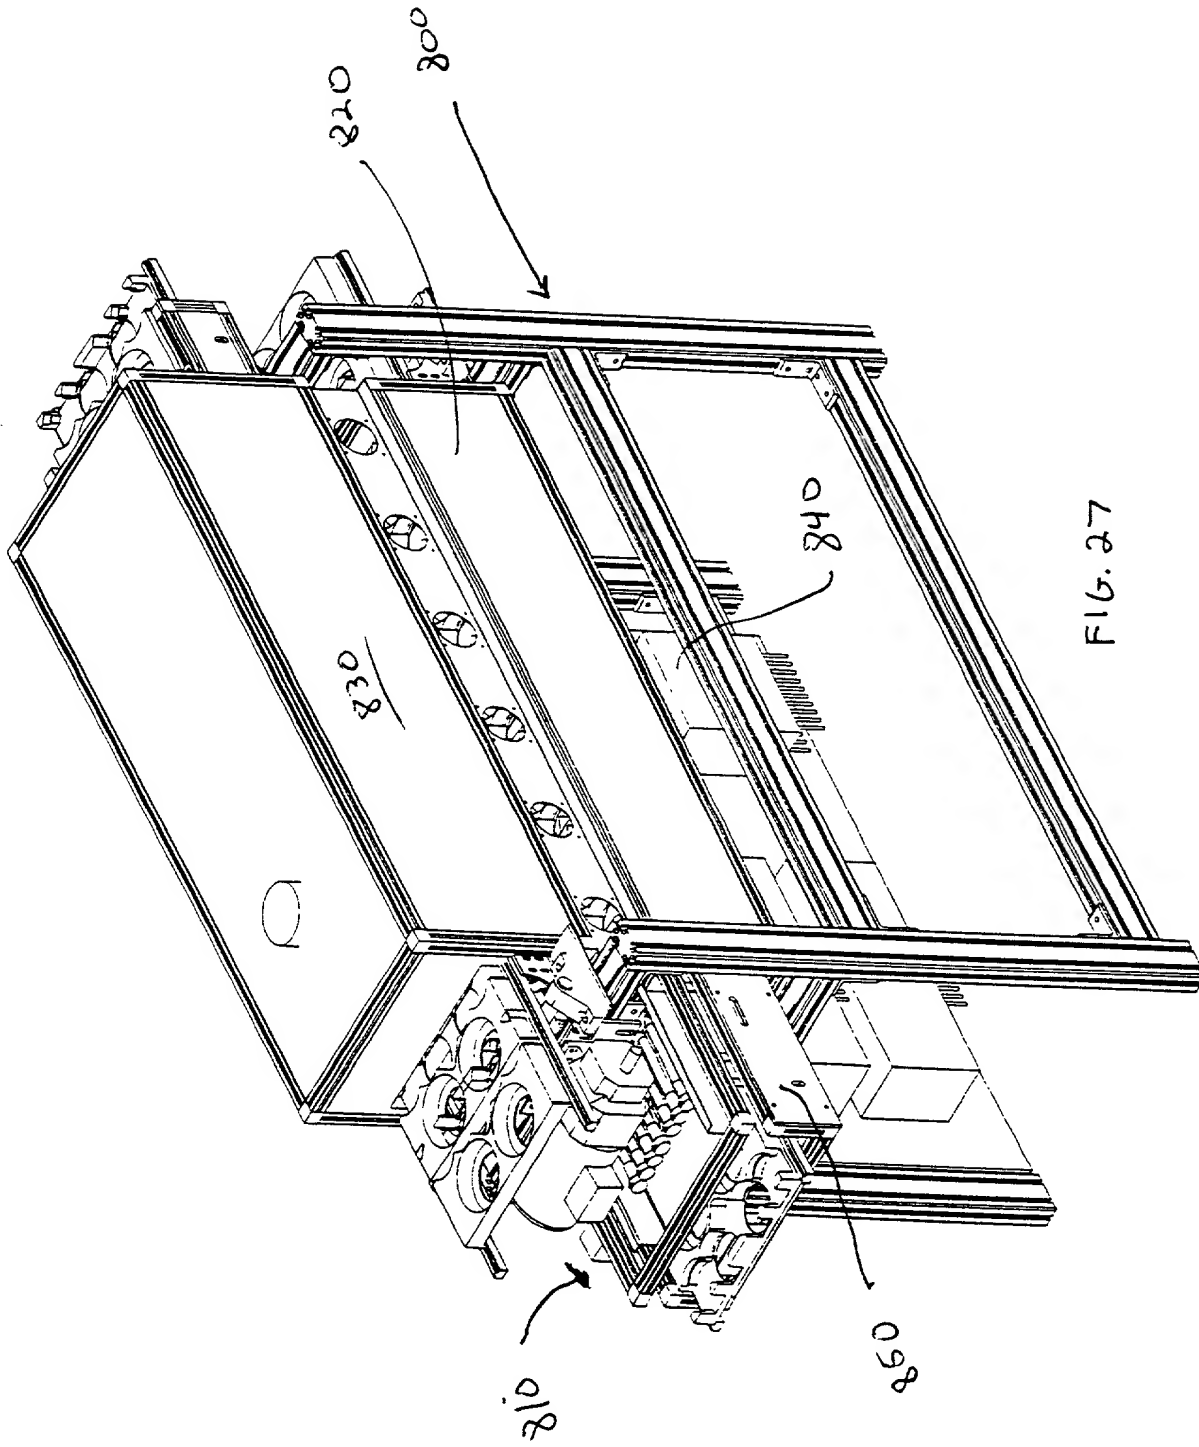


FIG. 27

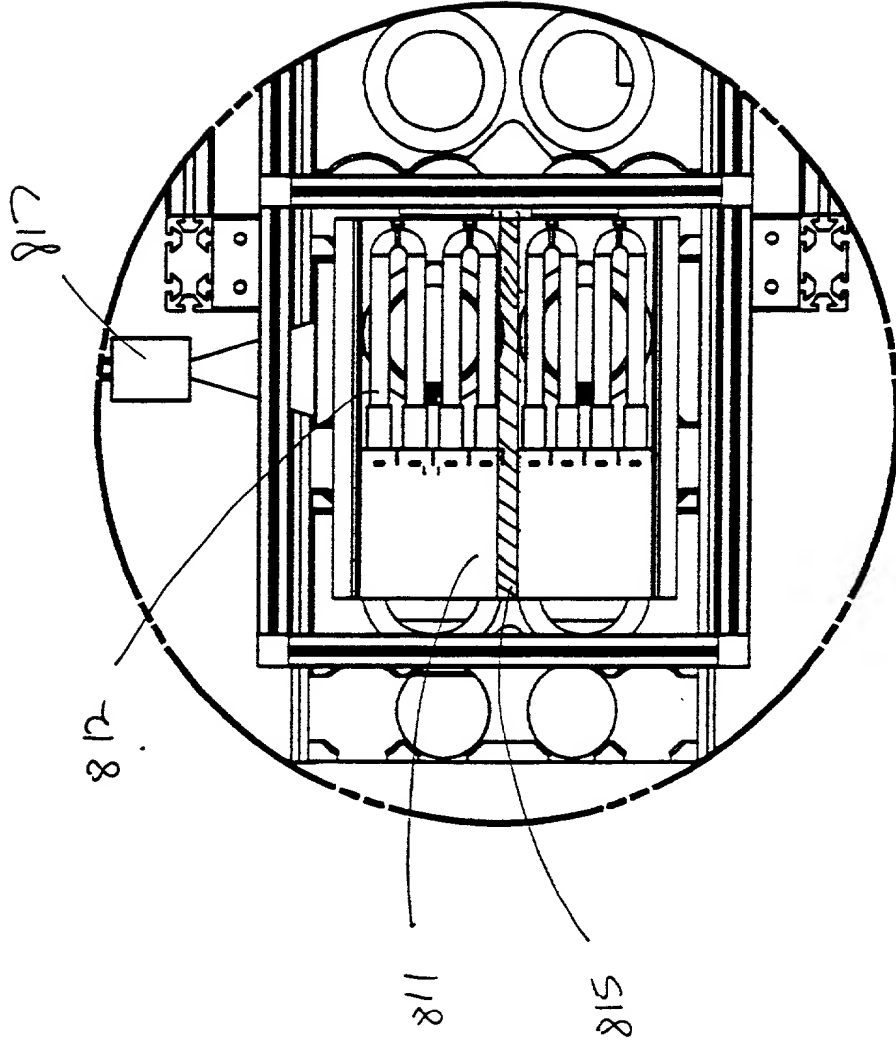


FIG. 29

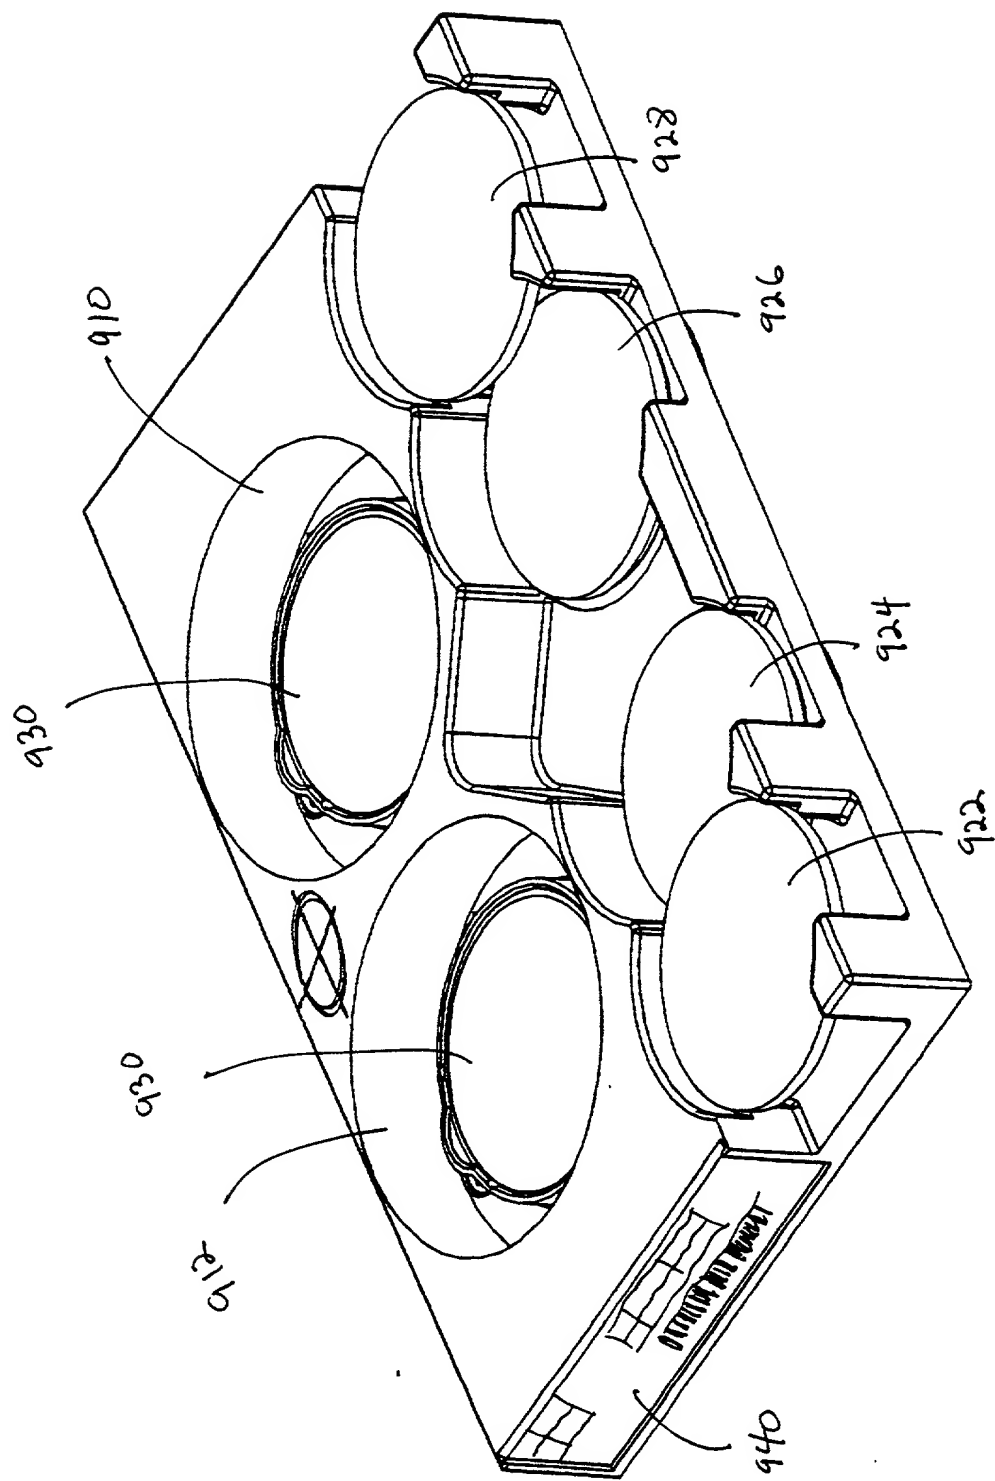


FIG. 30

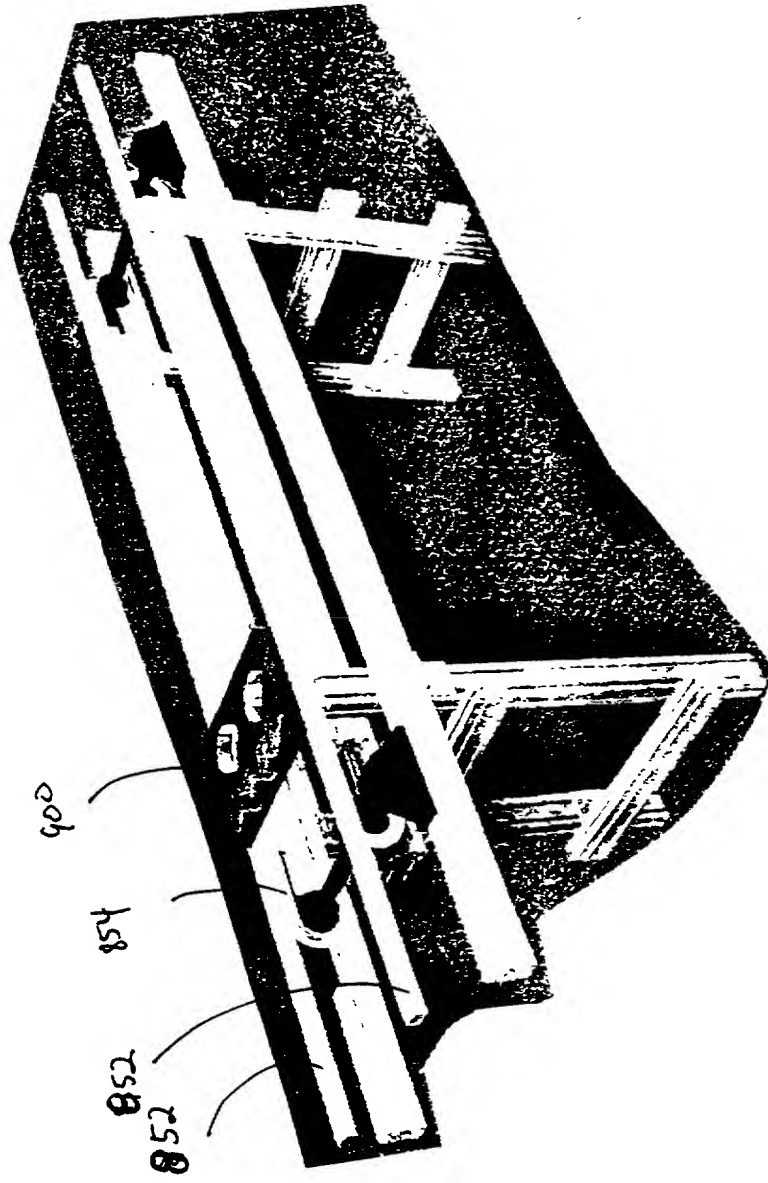


FIG. 31




Fig. 32

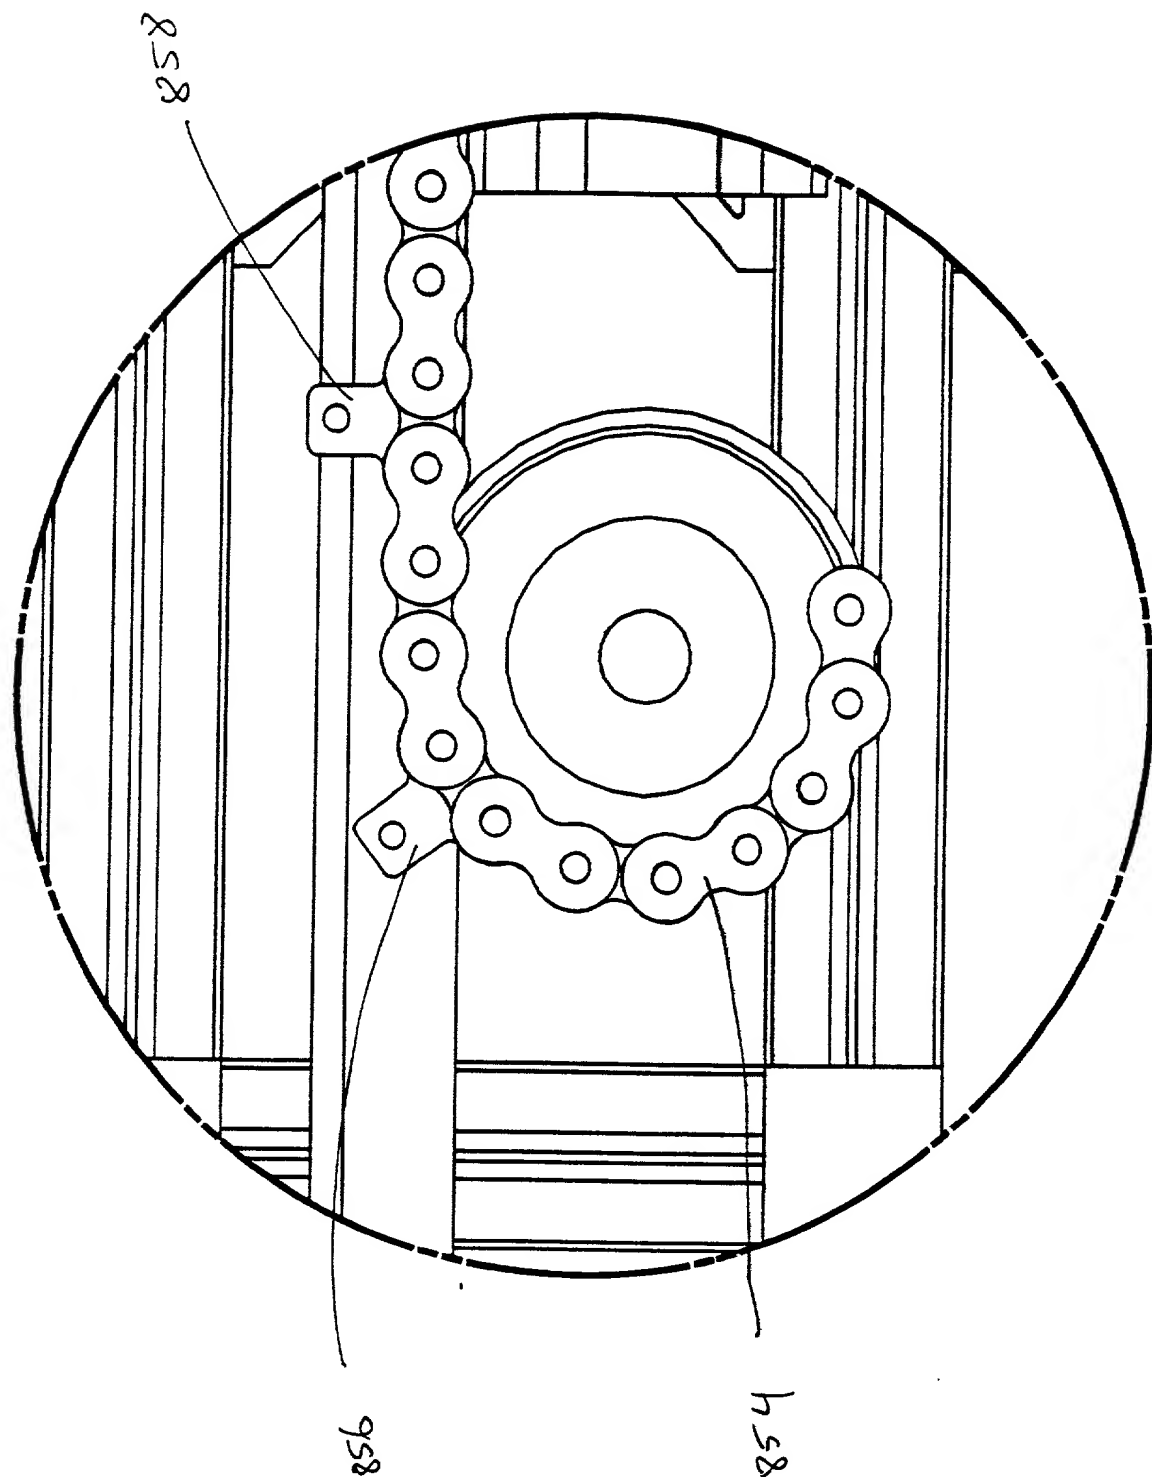


FIG. 33

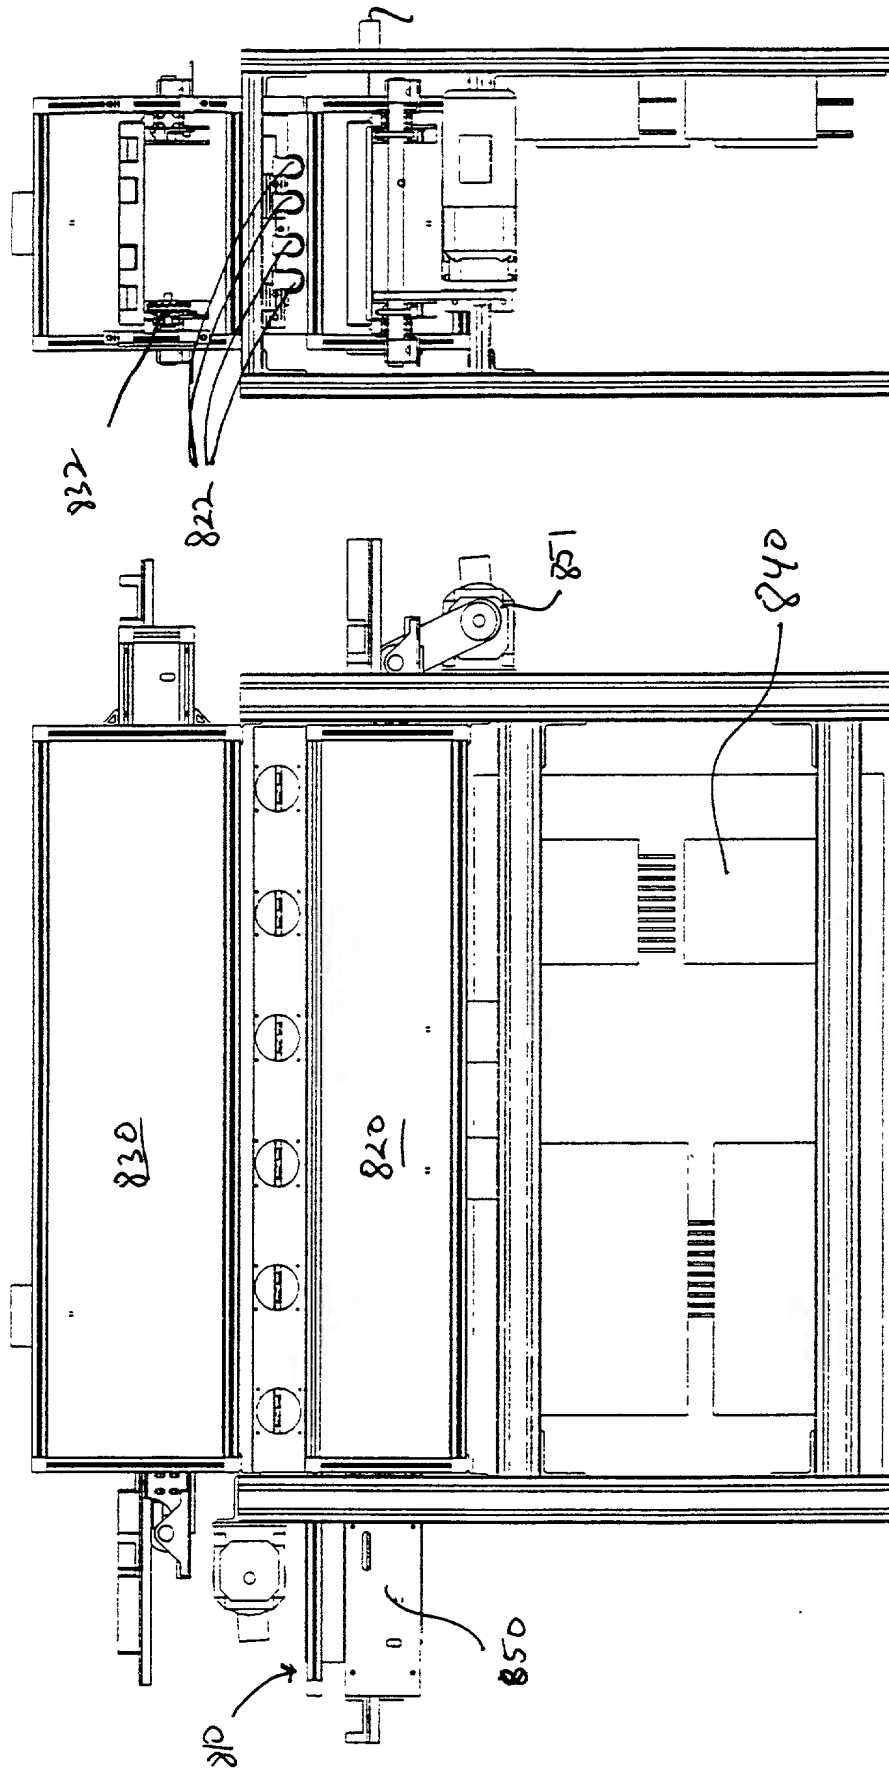


FIG. 34

FIG. 35



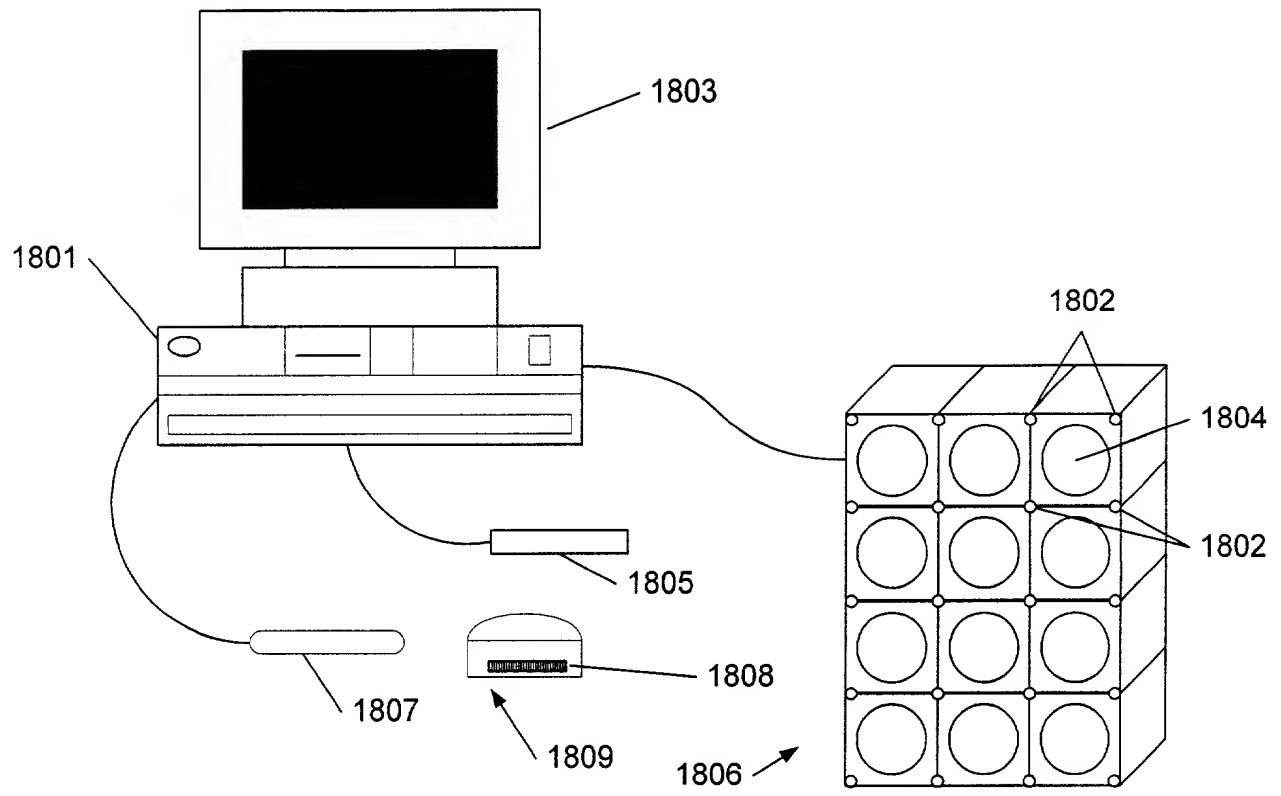


Fig.36

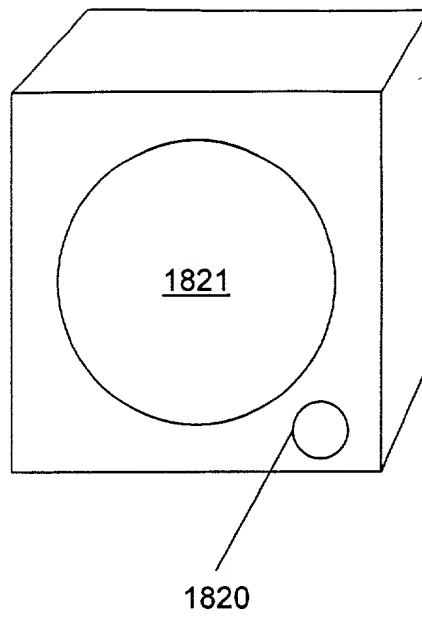

(a)

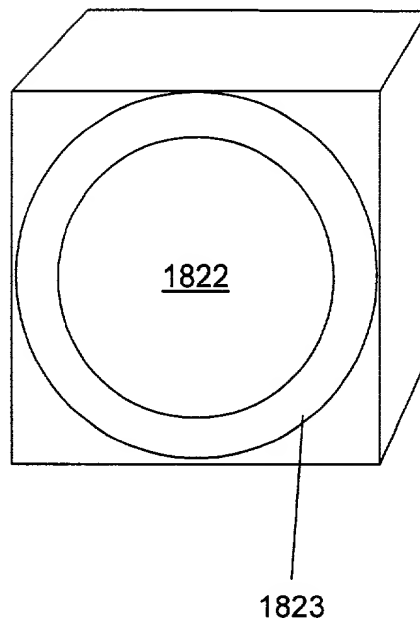

(b)

Fig. 37

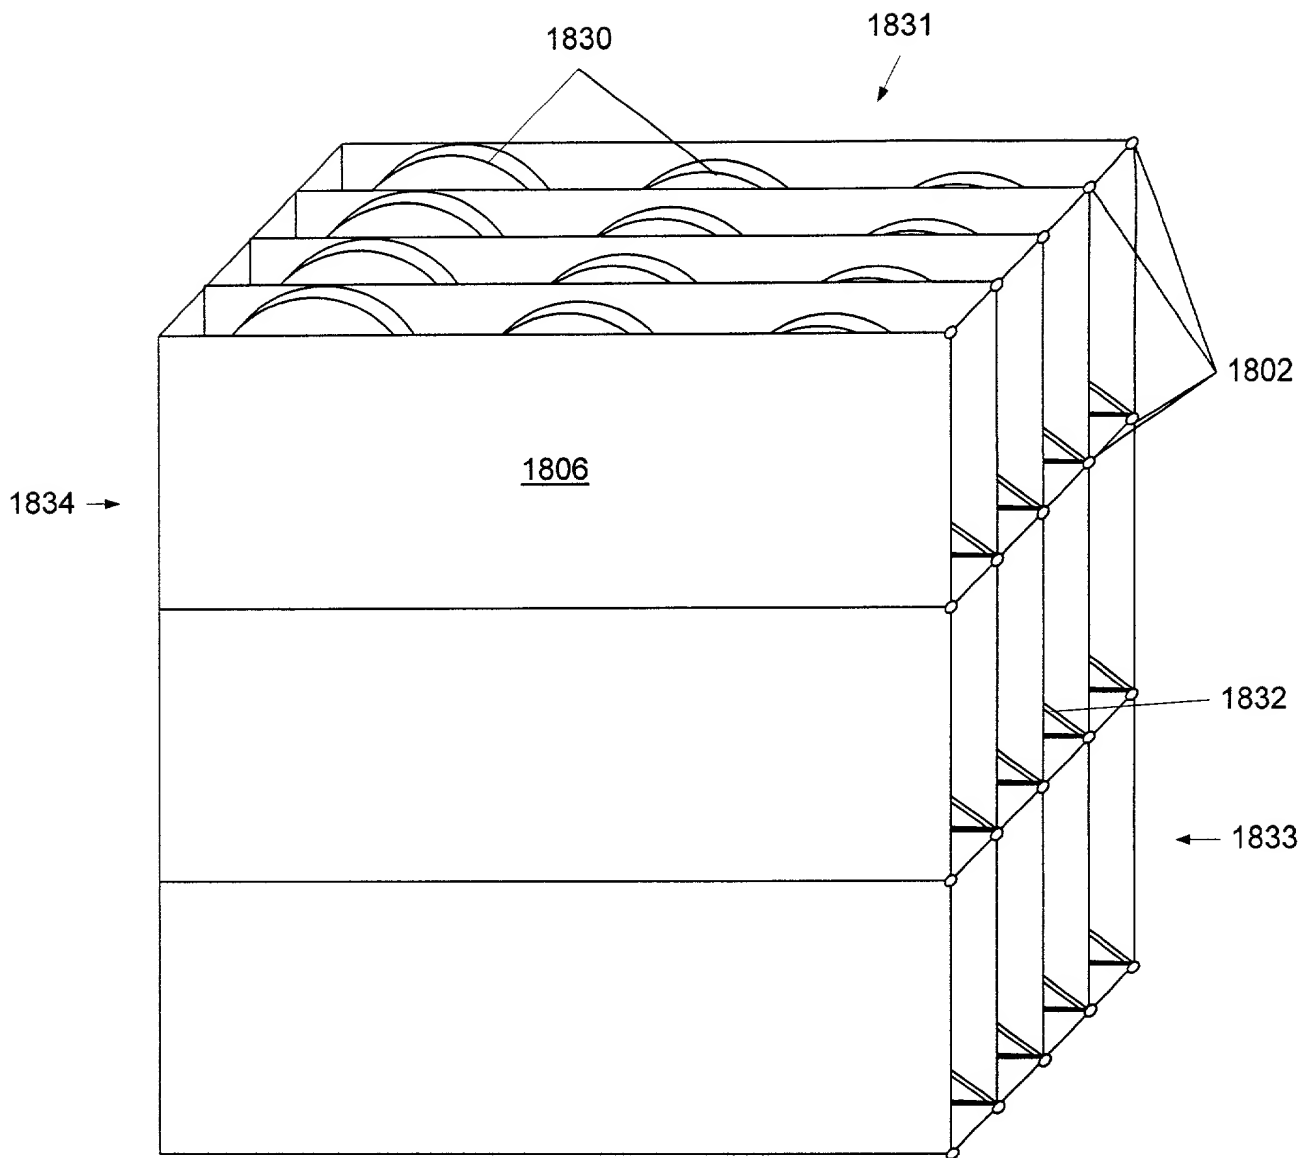


Fig. 38

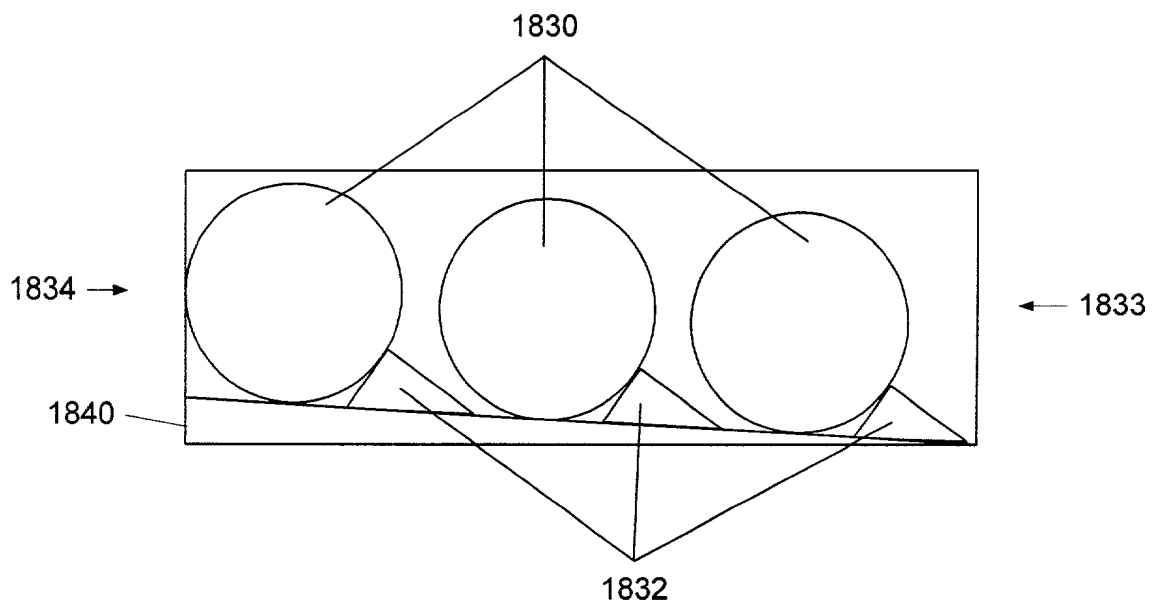


Fig. 39

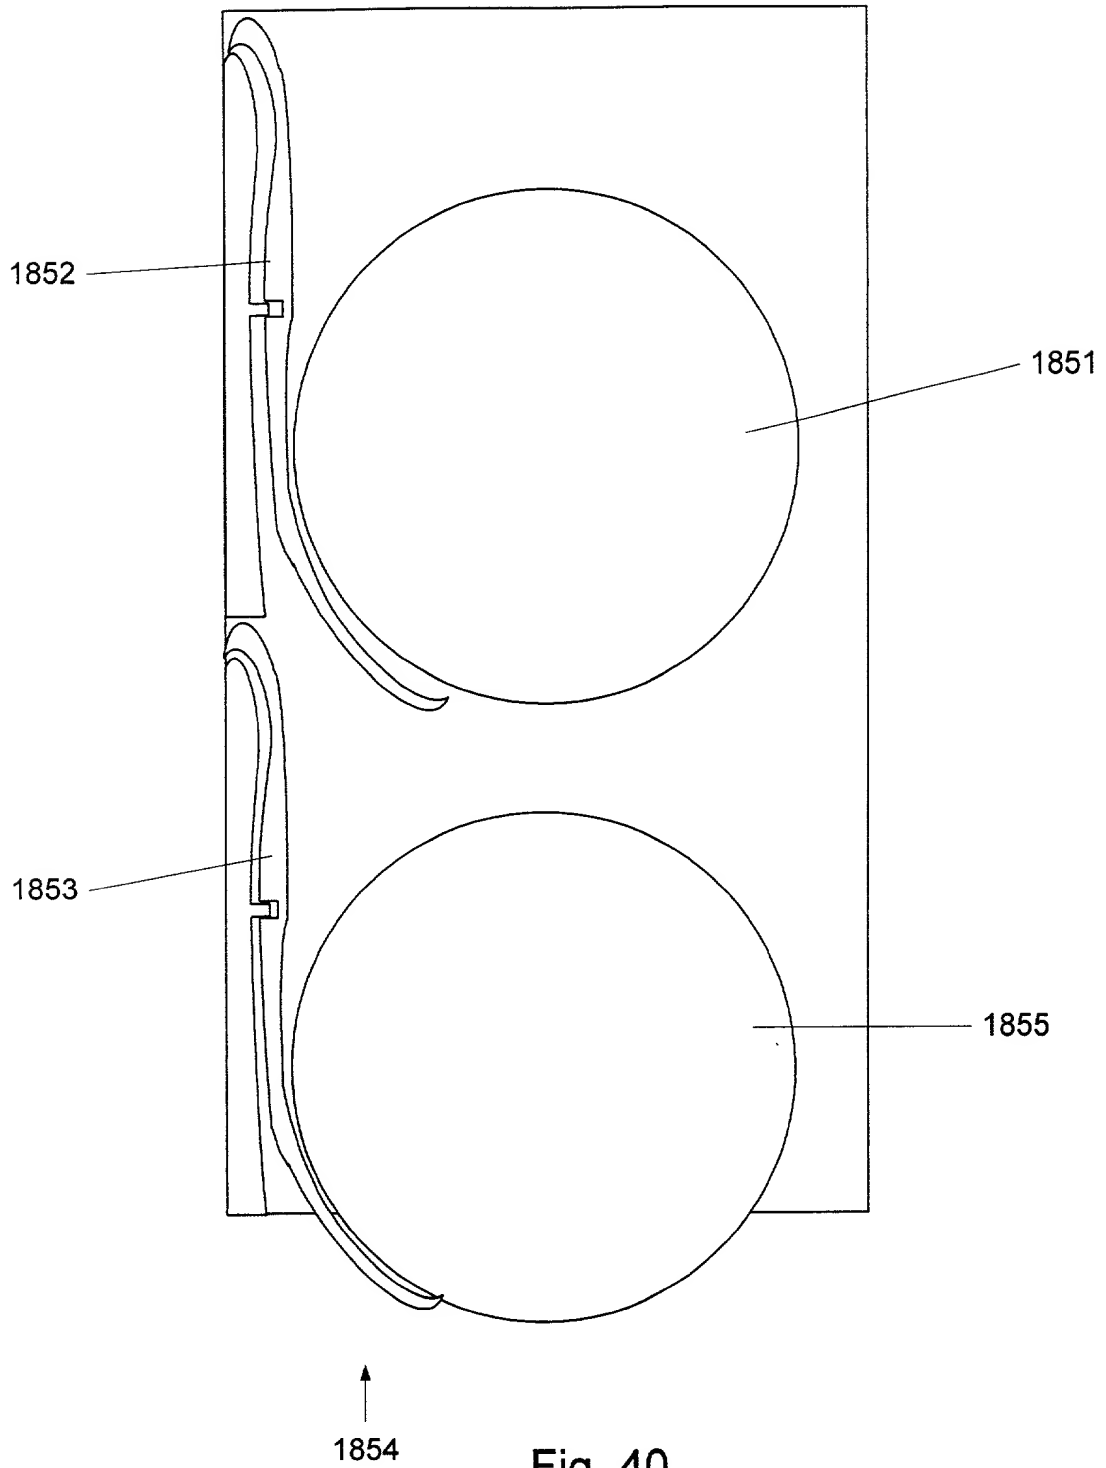


Fig. 40

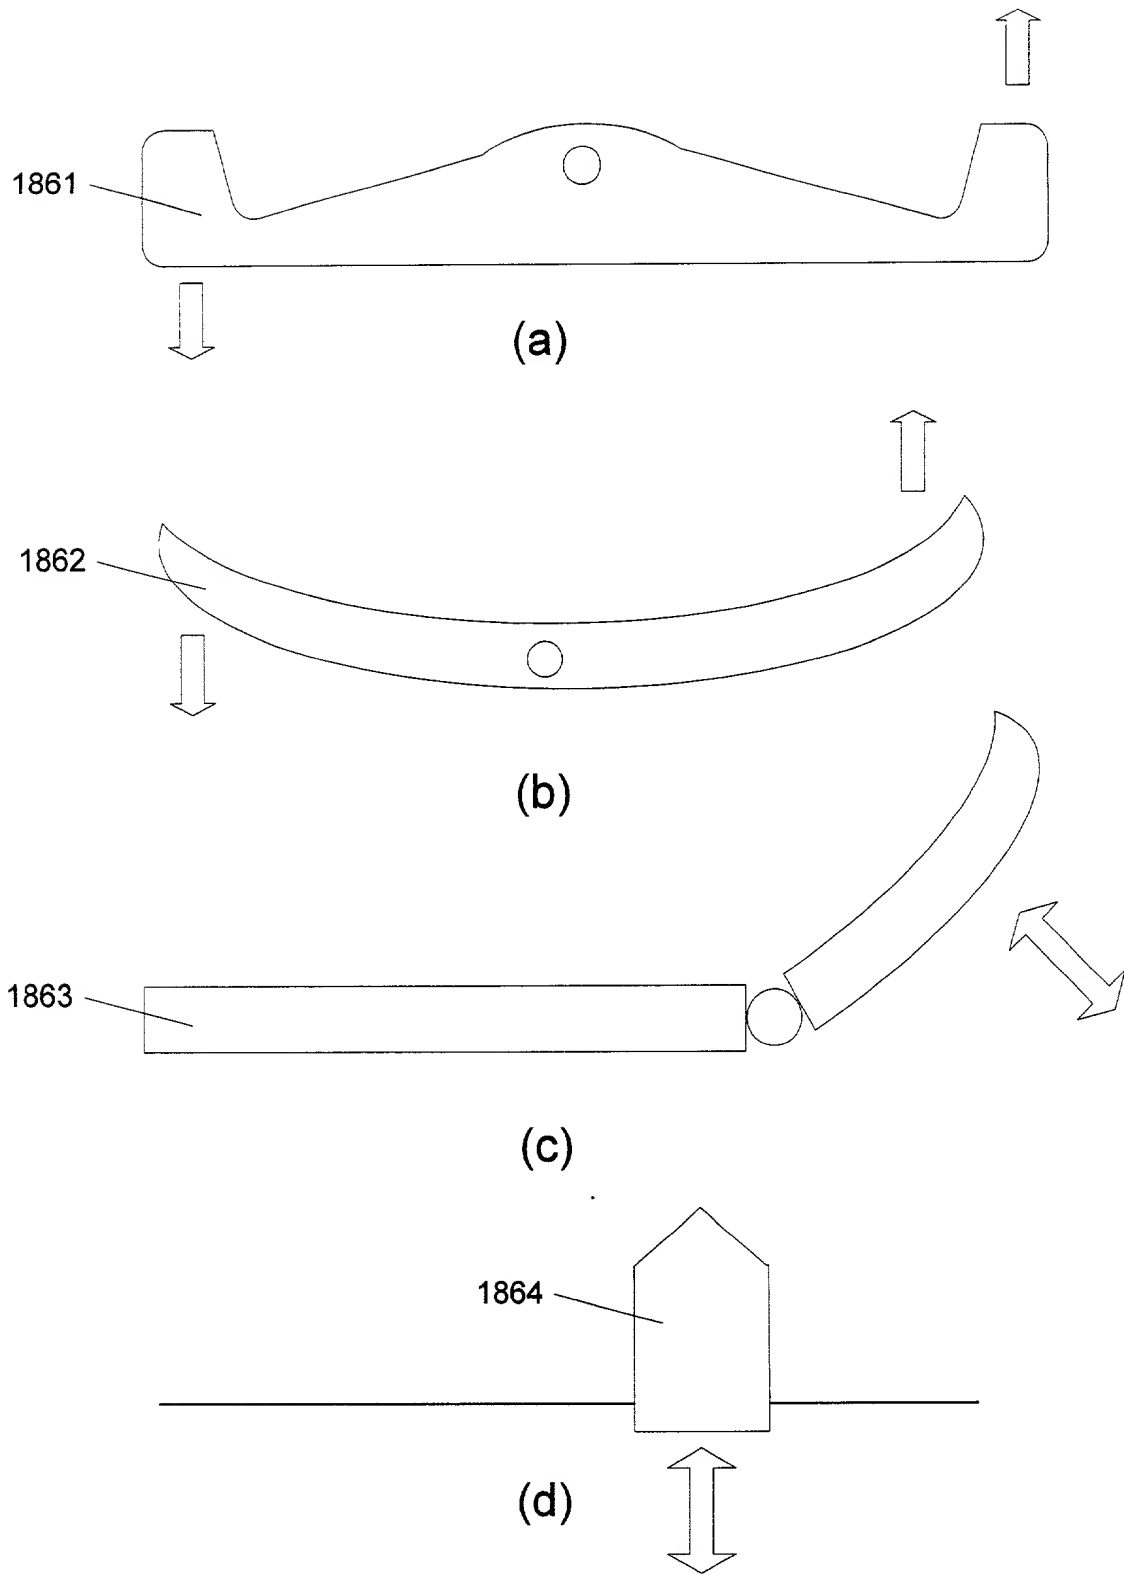


Fig. 41

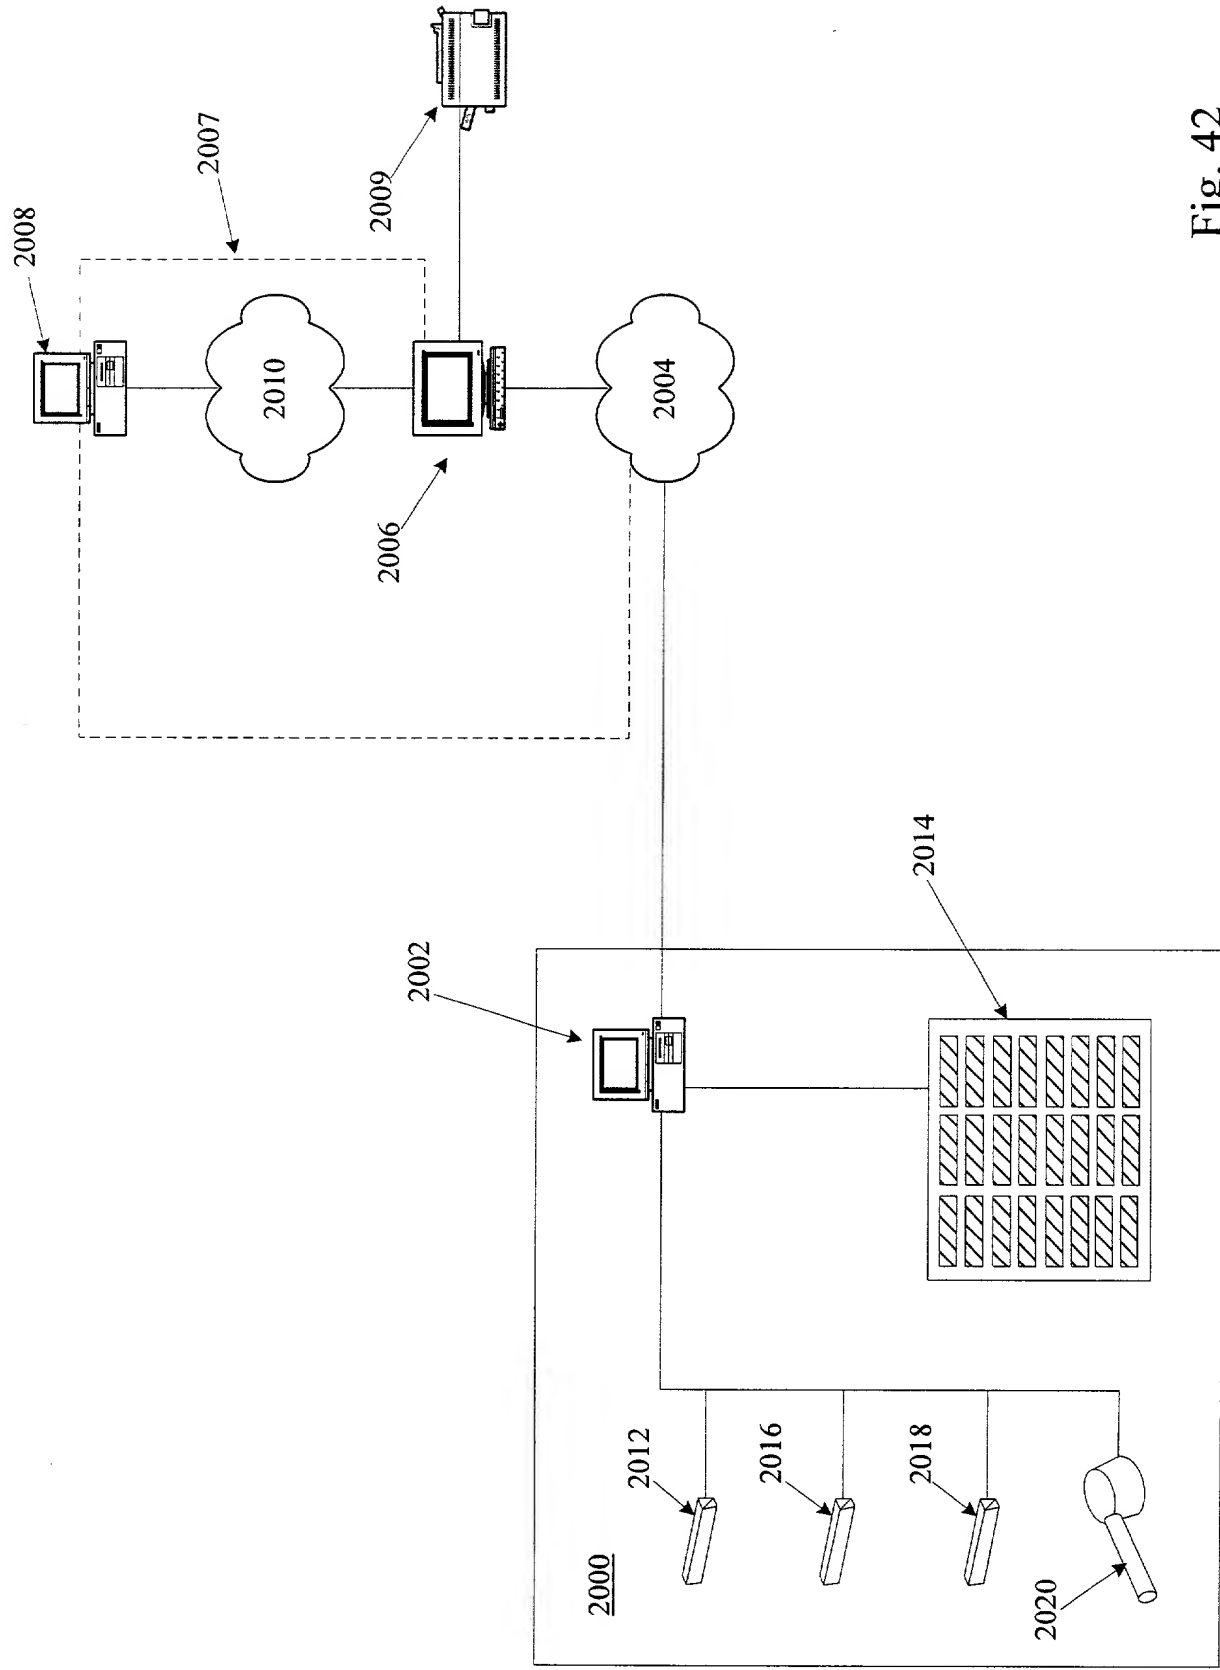


Fig. 42

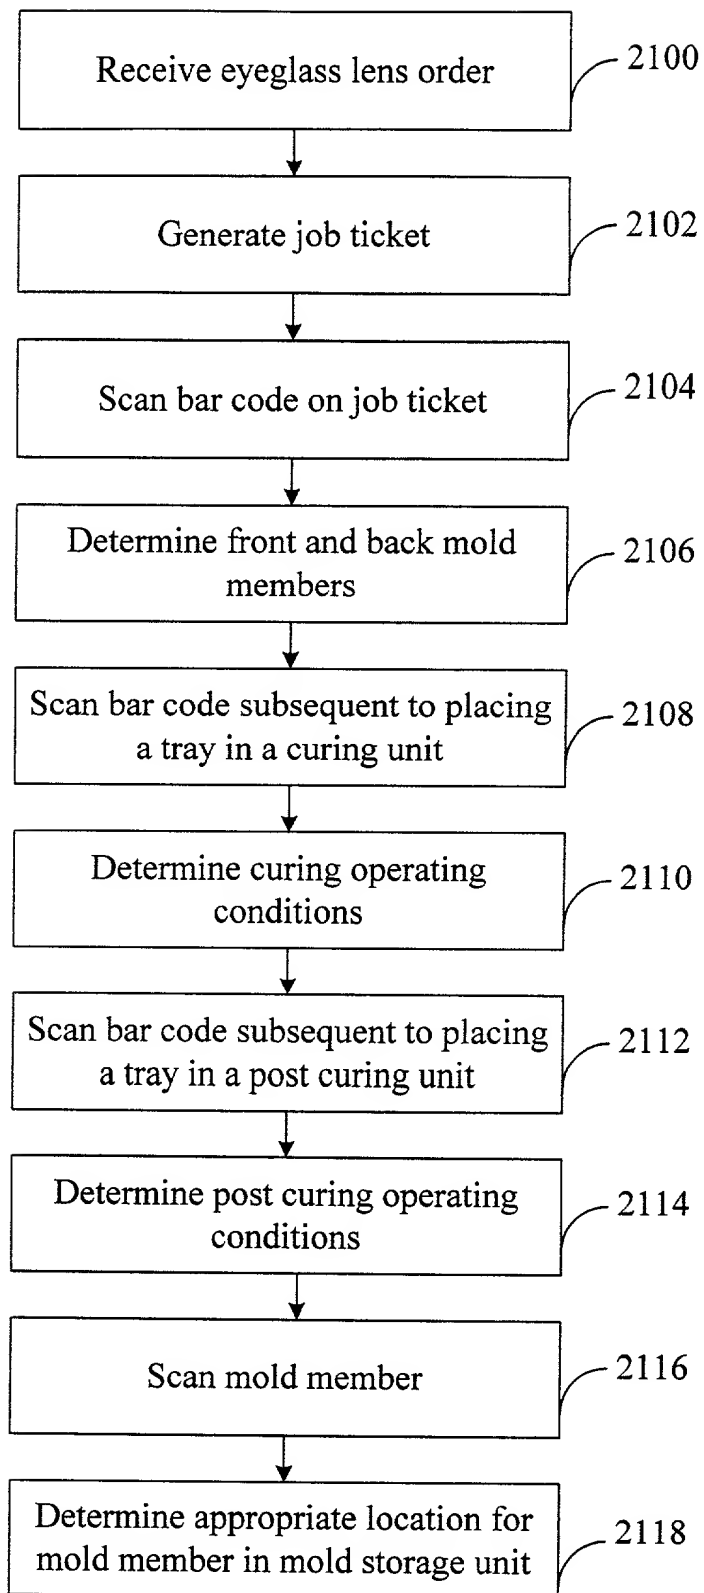


Fig. 43

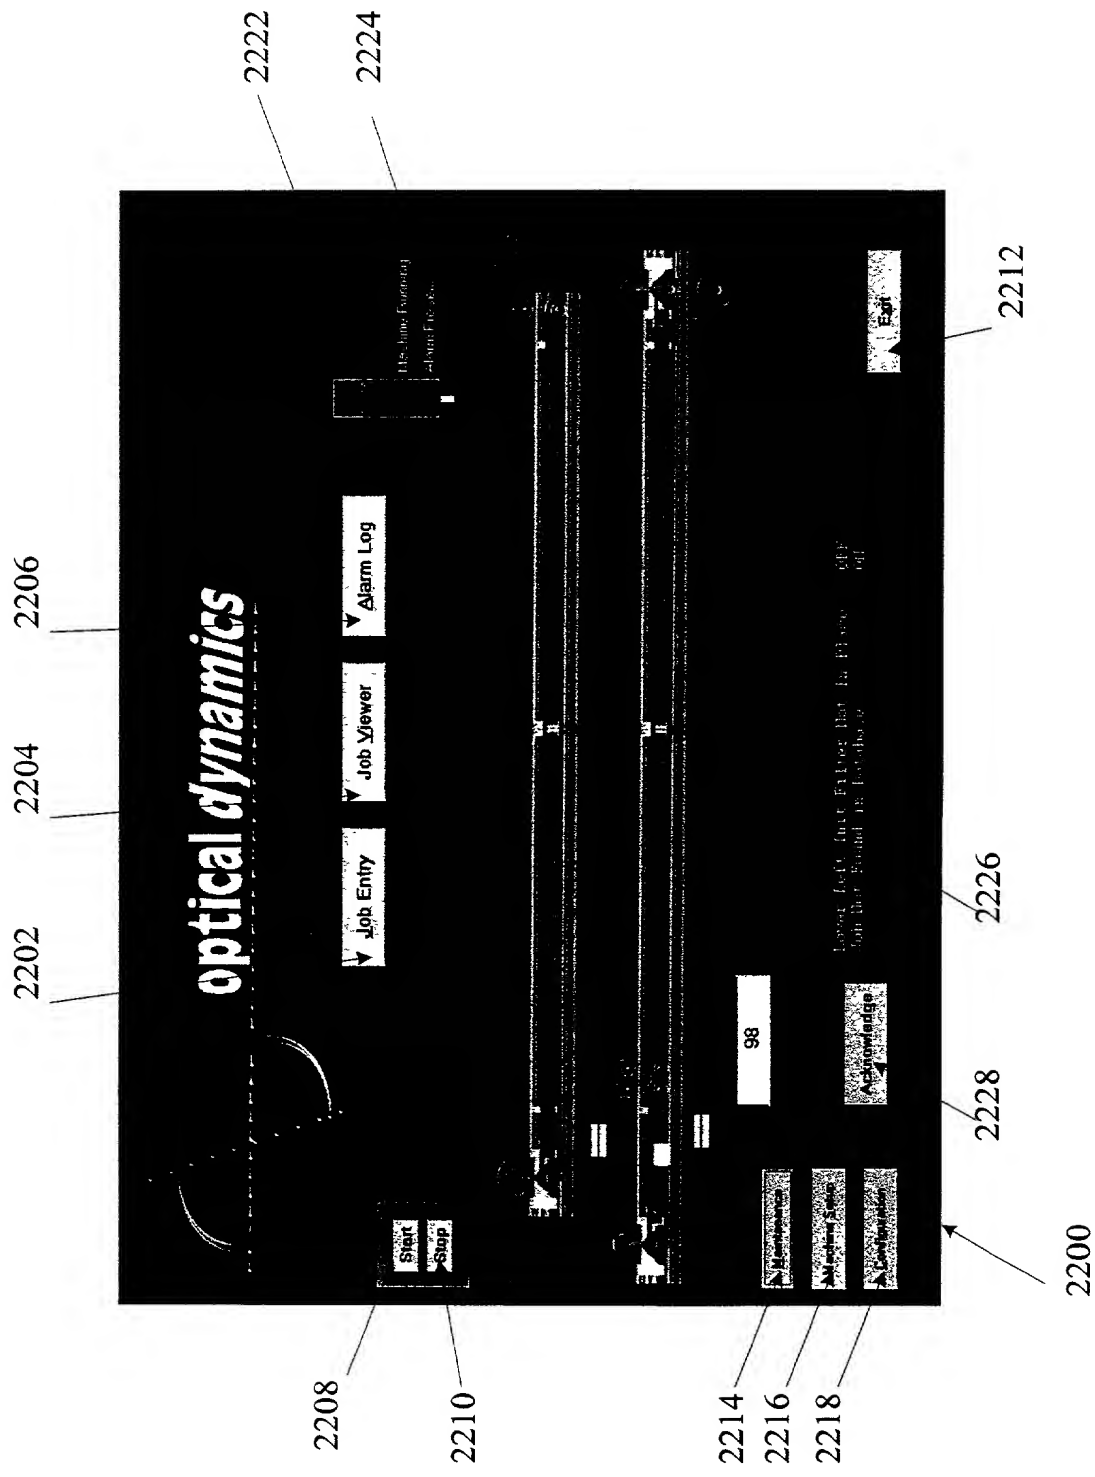


Fig. 44

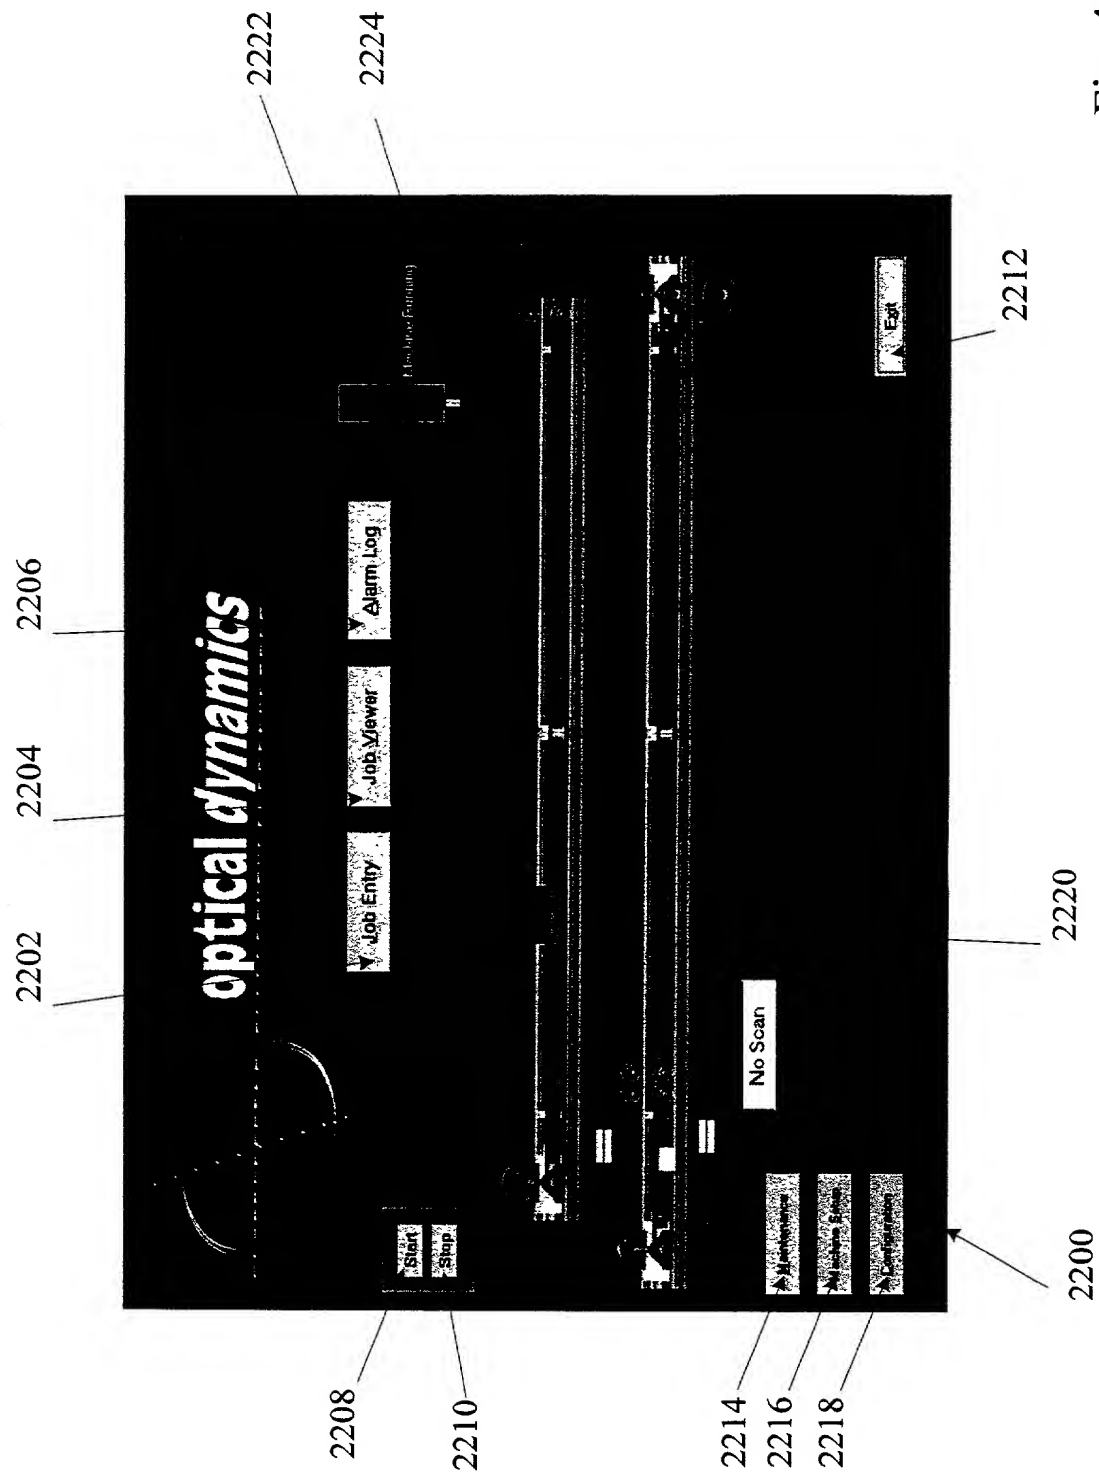


Fig. 45

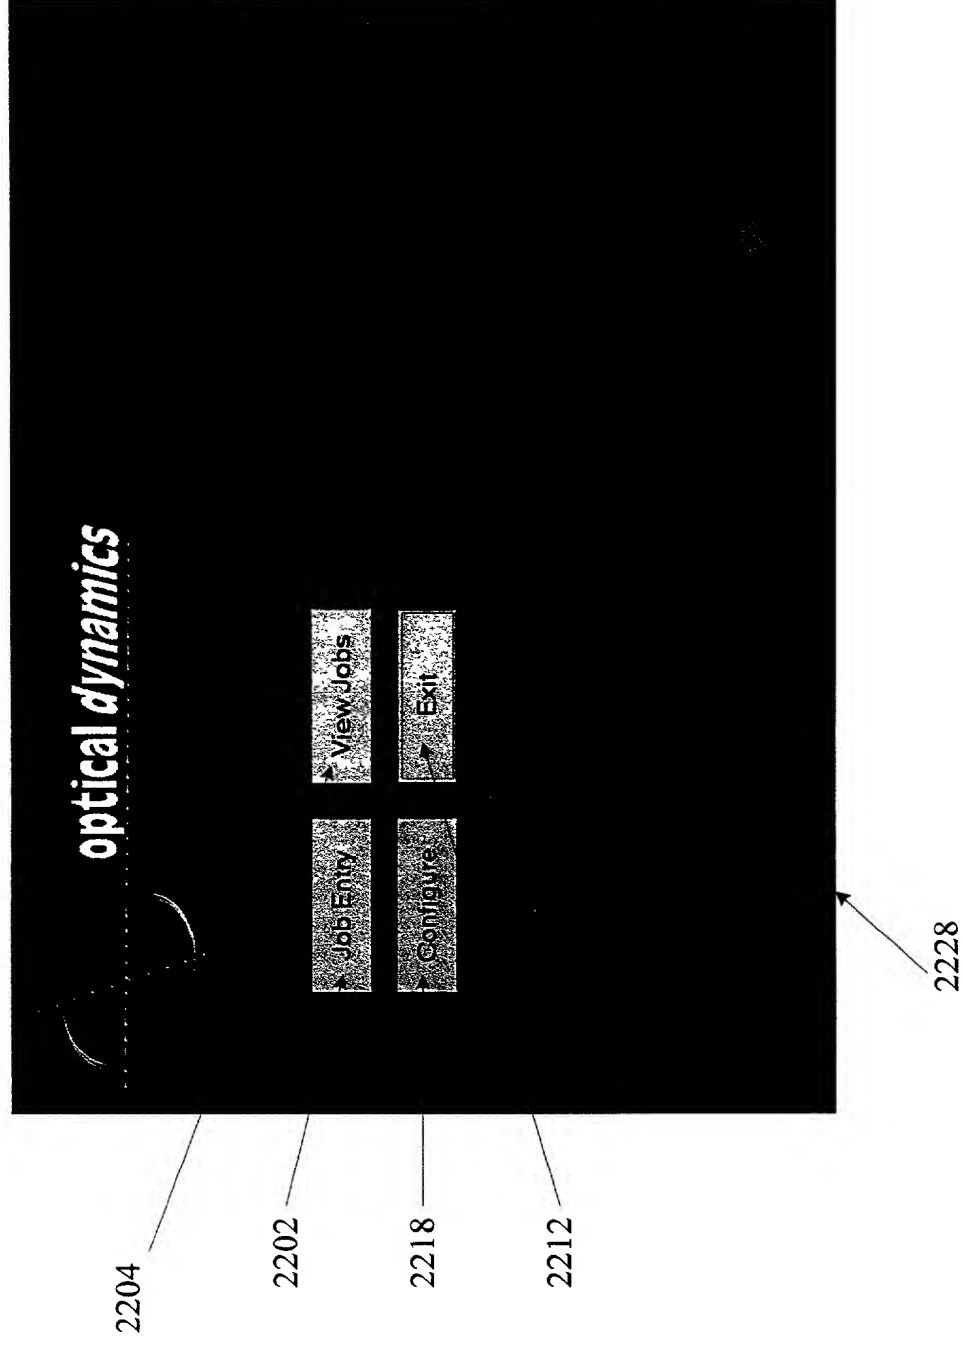


Fig. 46

2232

Job Entry

Job #

Patient Name

Tray #

Bin Location

Priority

Normal

Re-Work

Job Type

Right & Left Lens

Right Lens Only

Left Lens Only

Lens Type

Aspheric - Single Vision

Flat Top

Paradigm Progressive

Monomer/Tint

Clear

Clear w/ Tint

Grey

Right Eye

Sphere

Cylinder

Left Eye

Sphere

Cylinder

Cancel Entry

Create Job

2234

2236

2238

2240

2230

Fig. 47

Job Viewer

LMS Job #

LMS Tray #

Bin Location

Patient

Entry Date

Lens Type

Monomer

Rx

	Left	Right
Power	<input type="text" value="-6.00"/>	<input type="text"/>
Cylinder	<input type="text" value="-2.00"/>	<input type="text"/>
Axis	<input type="text"/>	<input type="text"/>
Add	<input type="text"/>	<input type="text"/>

Molds

	Left	Right
Front	<input type="text" value="No"/>	<input type="text"/>
Back	<input type="text" value="Rx"/>	<input type="text"/>
Gasket	<input type="text" value="Mold"/>	<input type="text"/>
Filter	<input type="text"/>	<input type="text"/>
Recipe	<input type="text"/>	<input type="text"/>

Transposed

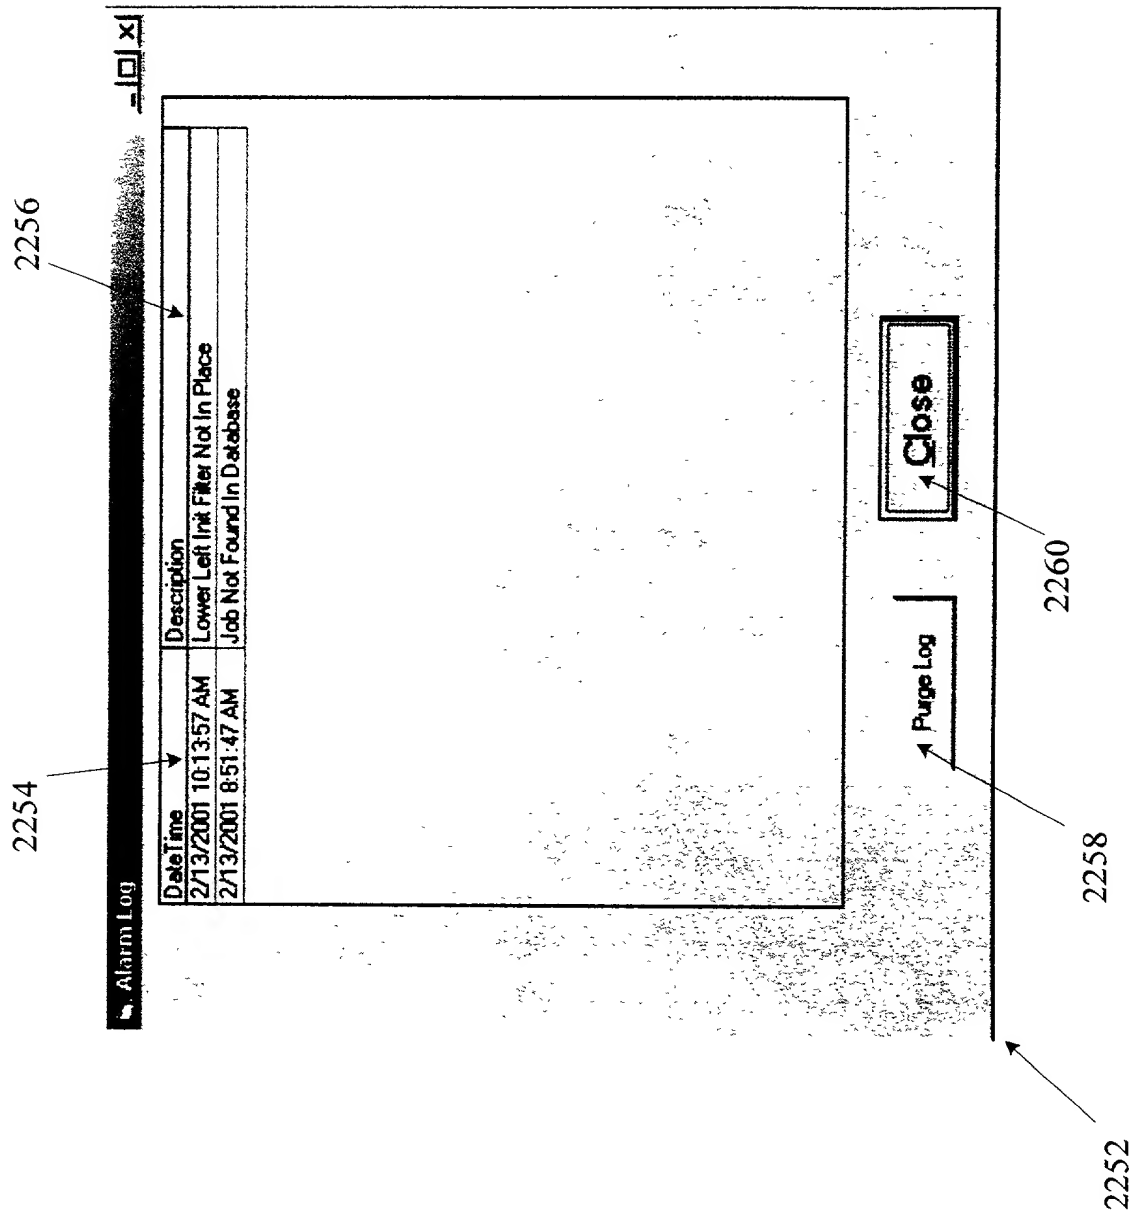


Fig. 49

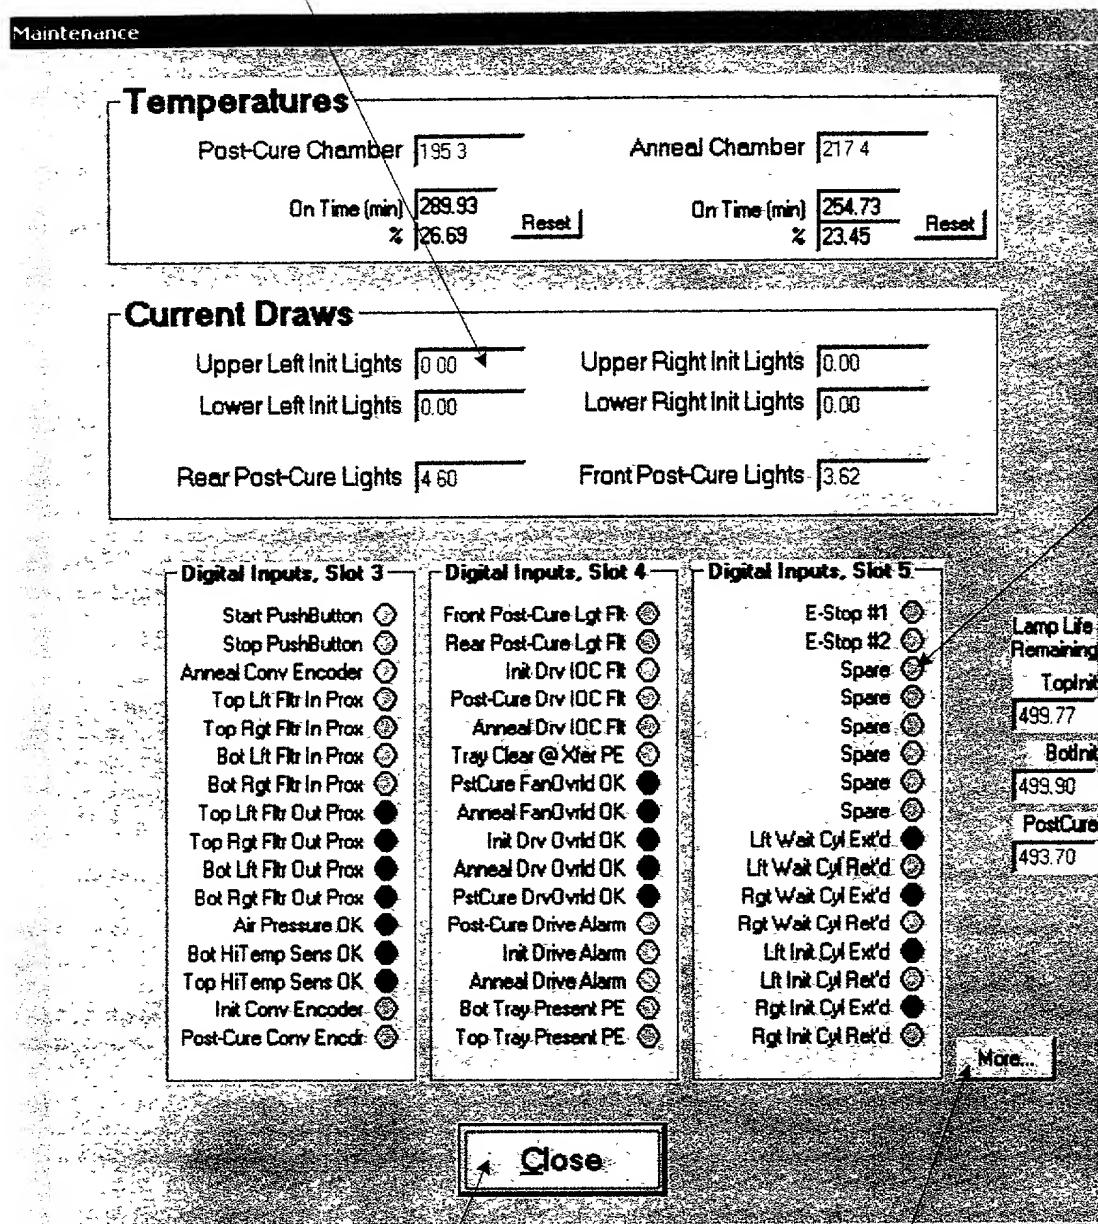


Fig. 50

Machine Setup

Anneal Conveyor

High Temp Alarm Limit

Temperature Setpoint

Low Temp Alarm Limit

Post-Cure Conveyor

High Temp Alarm Limit

Temperature Setpoint

Low Temp Alarm Limit

Initialization Lights

High Current Alarm Limit

Low Current Alarm Limit

No Scan Upper Init Time

No Scan Lower Init Time

No Scan Filter Select ☐

Post-Cure Lights

High Current Alarm Limit

Low Current Alarm Limit

Lamp Maintenance

Replaced Top Init Lamps ☐

Replaced Bot Init Lamps ☐

Replaced Post-Cure Lamps ☐

Save Changes **Cancel Changes**

2274

2272

2278

2280

2276

Fig. 51

2282

Recipe DB: C:\OptDyn\MGR112700.mdb Browse... 2284 2286 2288

Job DB: C:\OptDyn\JobTickets.mdb Browse... 2290

Ticket Dir: C:\OptDyn\ Browse... 2292

Ticket Poll Rate (sec) 2 2294

Ticket Print Scale (%) 100

Archive Jobs Every 14 Days Keeping 3 Days

Cancel OK

Fig. 52

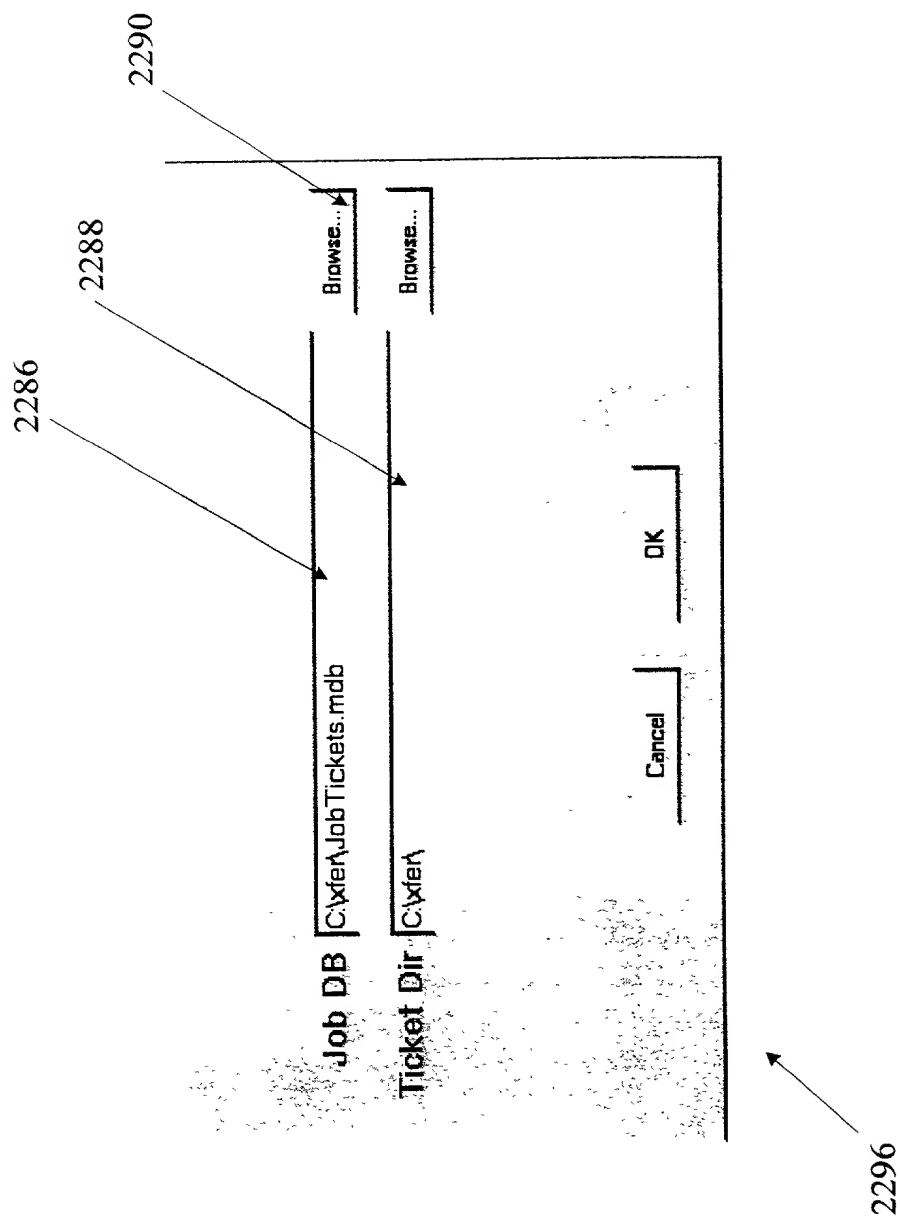


Fig. 53